Measurement Results vs Spike Concentrations (Log-10 Scale)

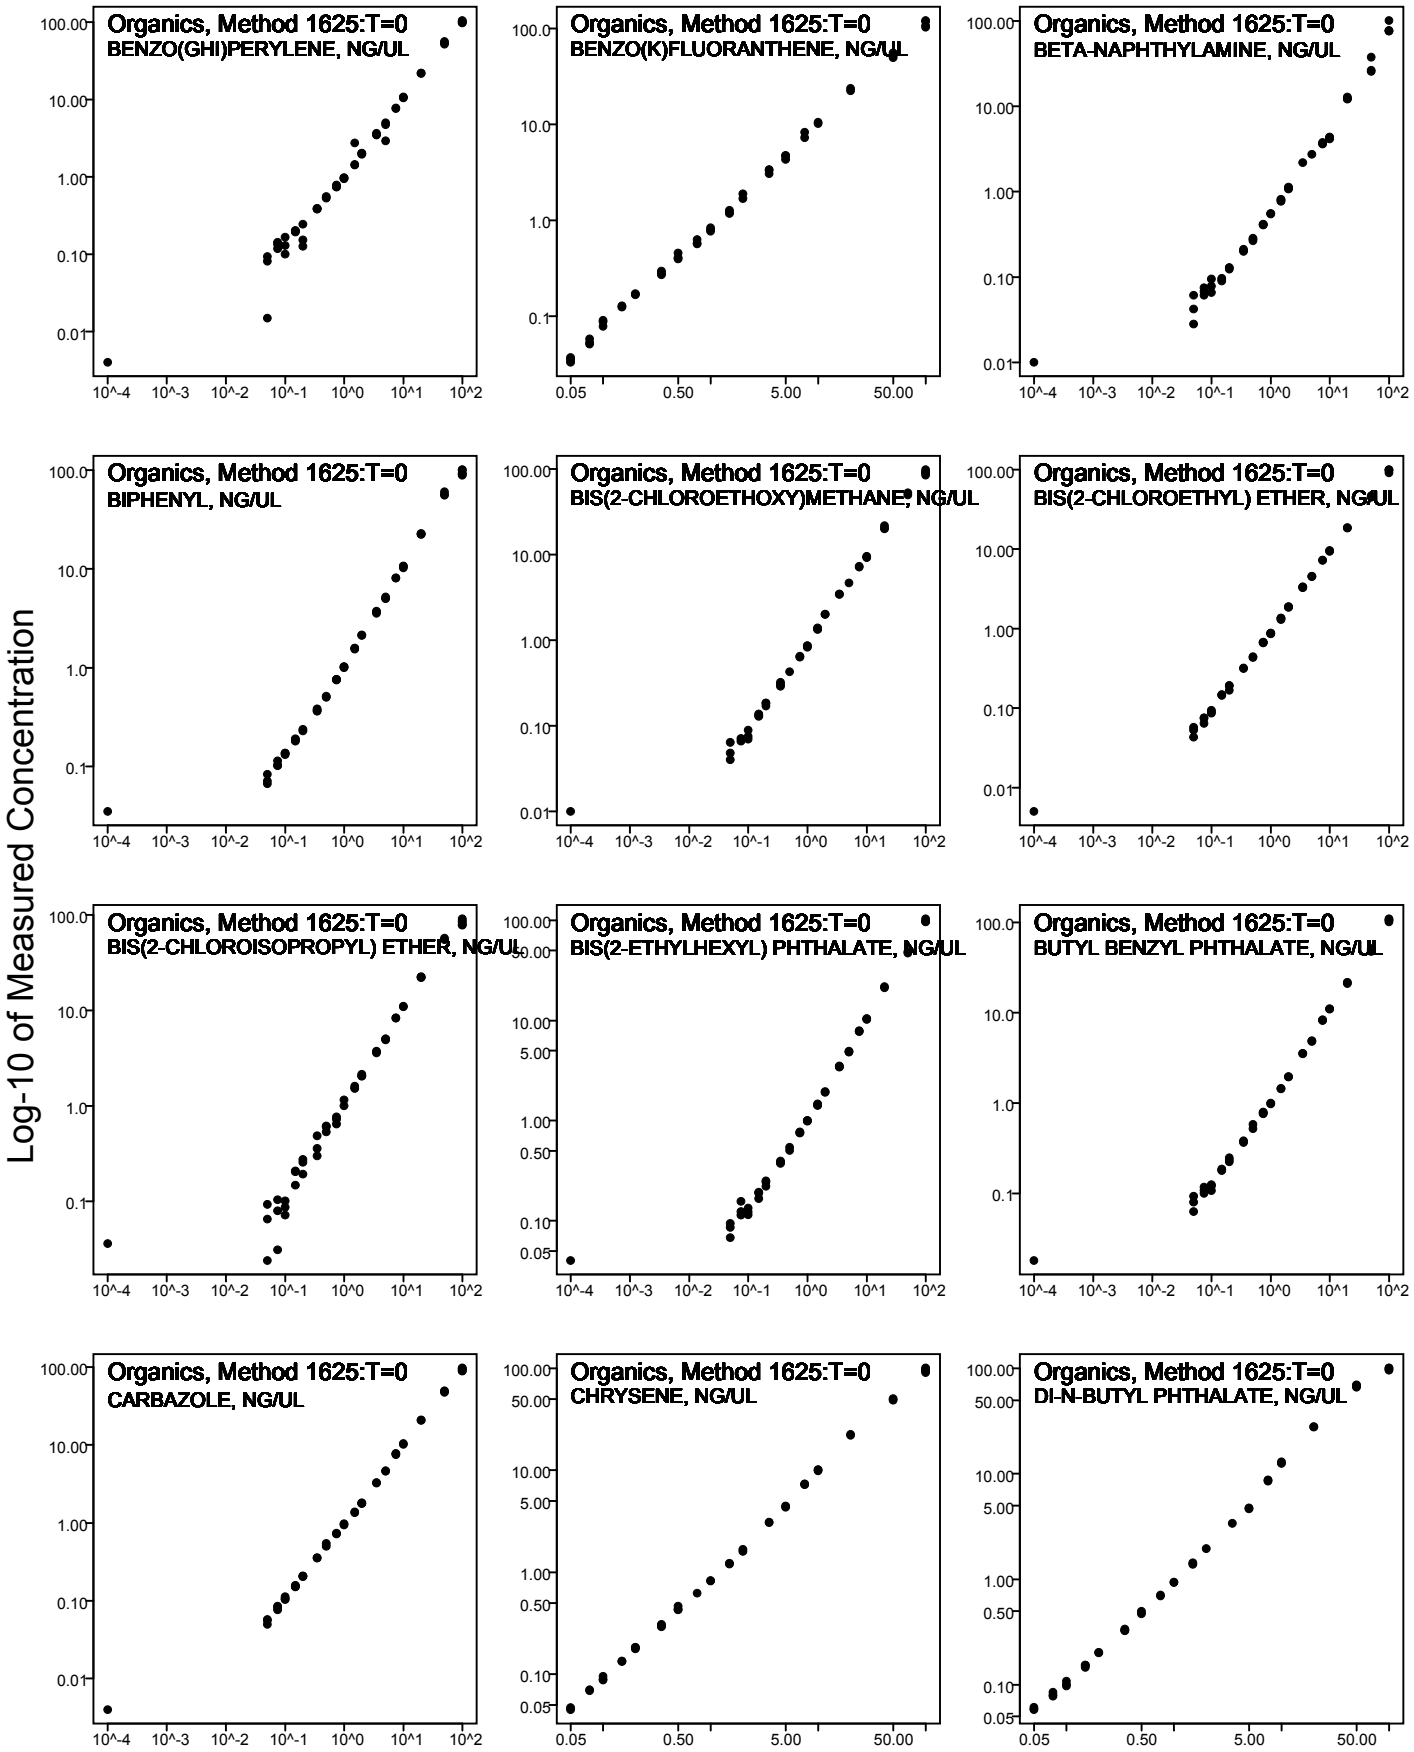

Measurement Results vs Spike Concentrations (Log-10 Scale)

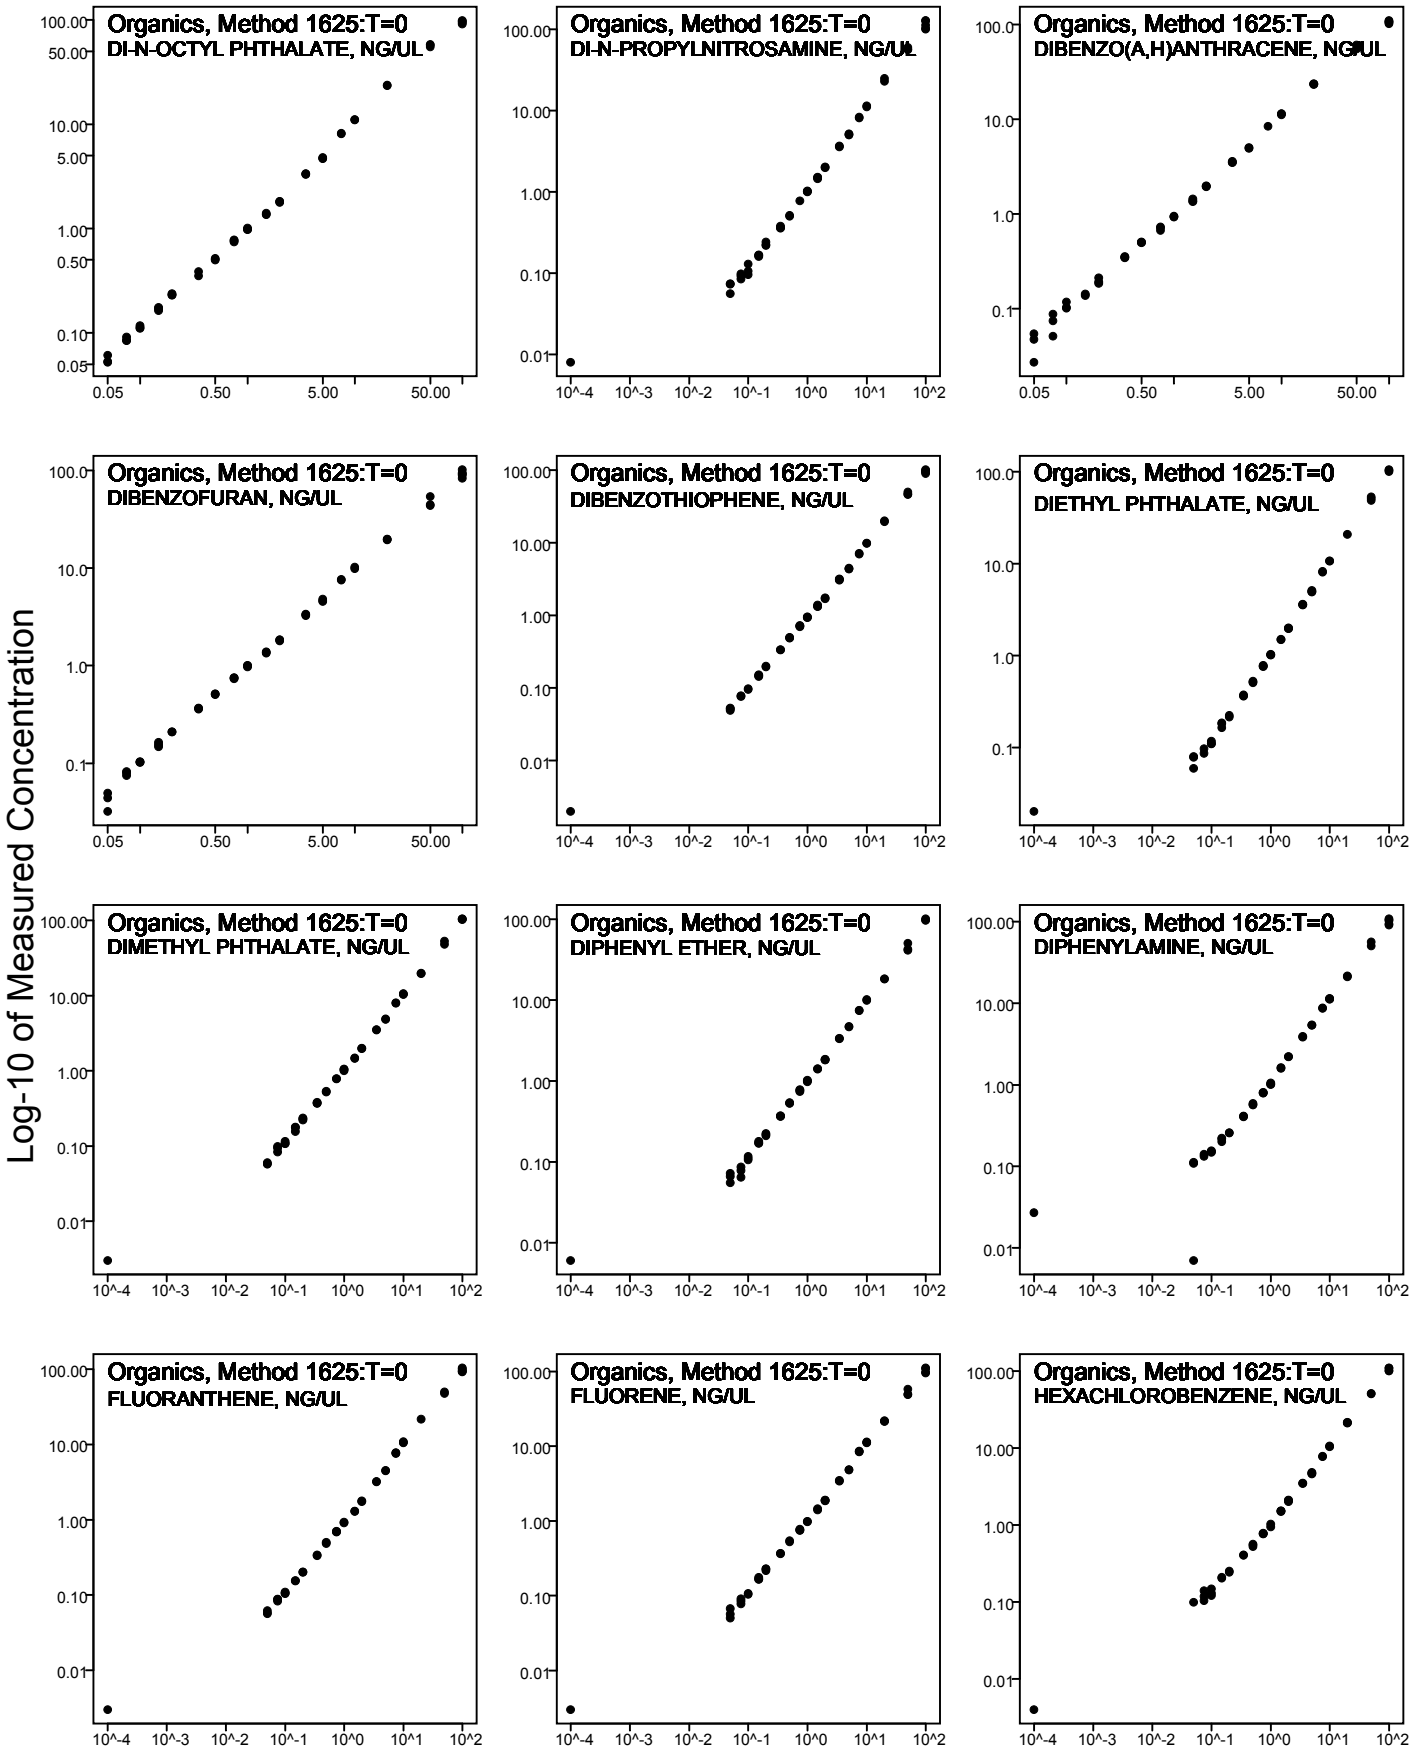

Measurement Results vs Spike Concentrations (Log-10 Scale)

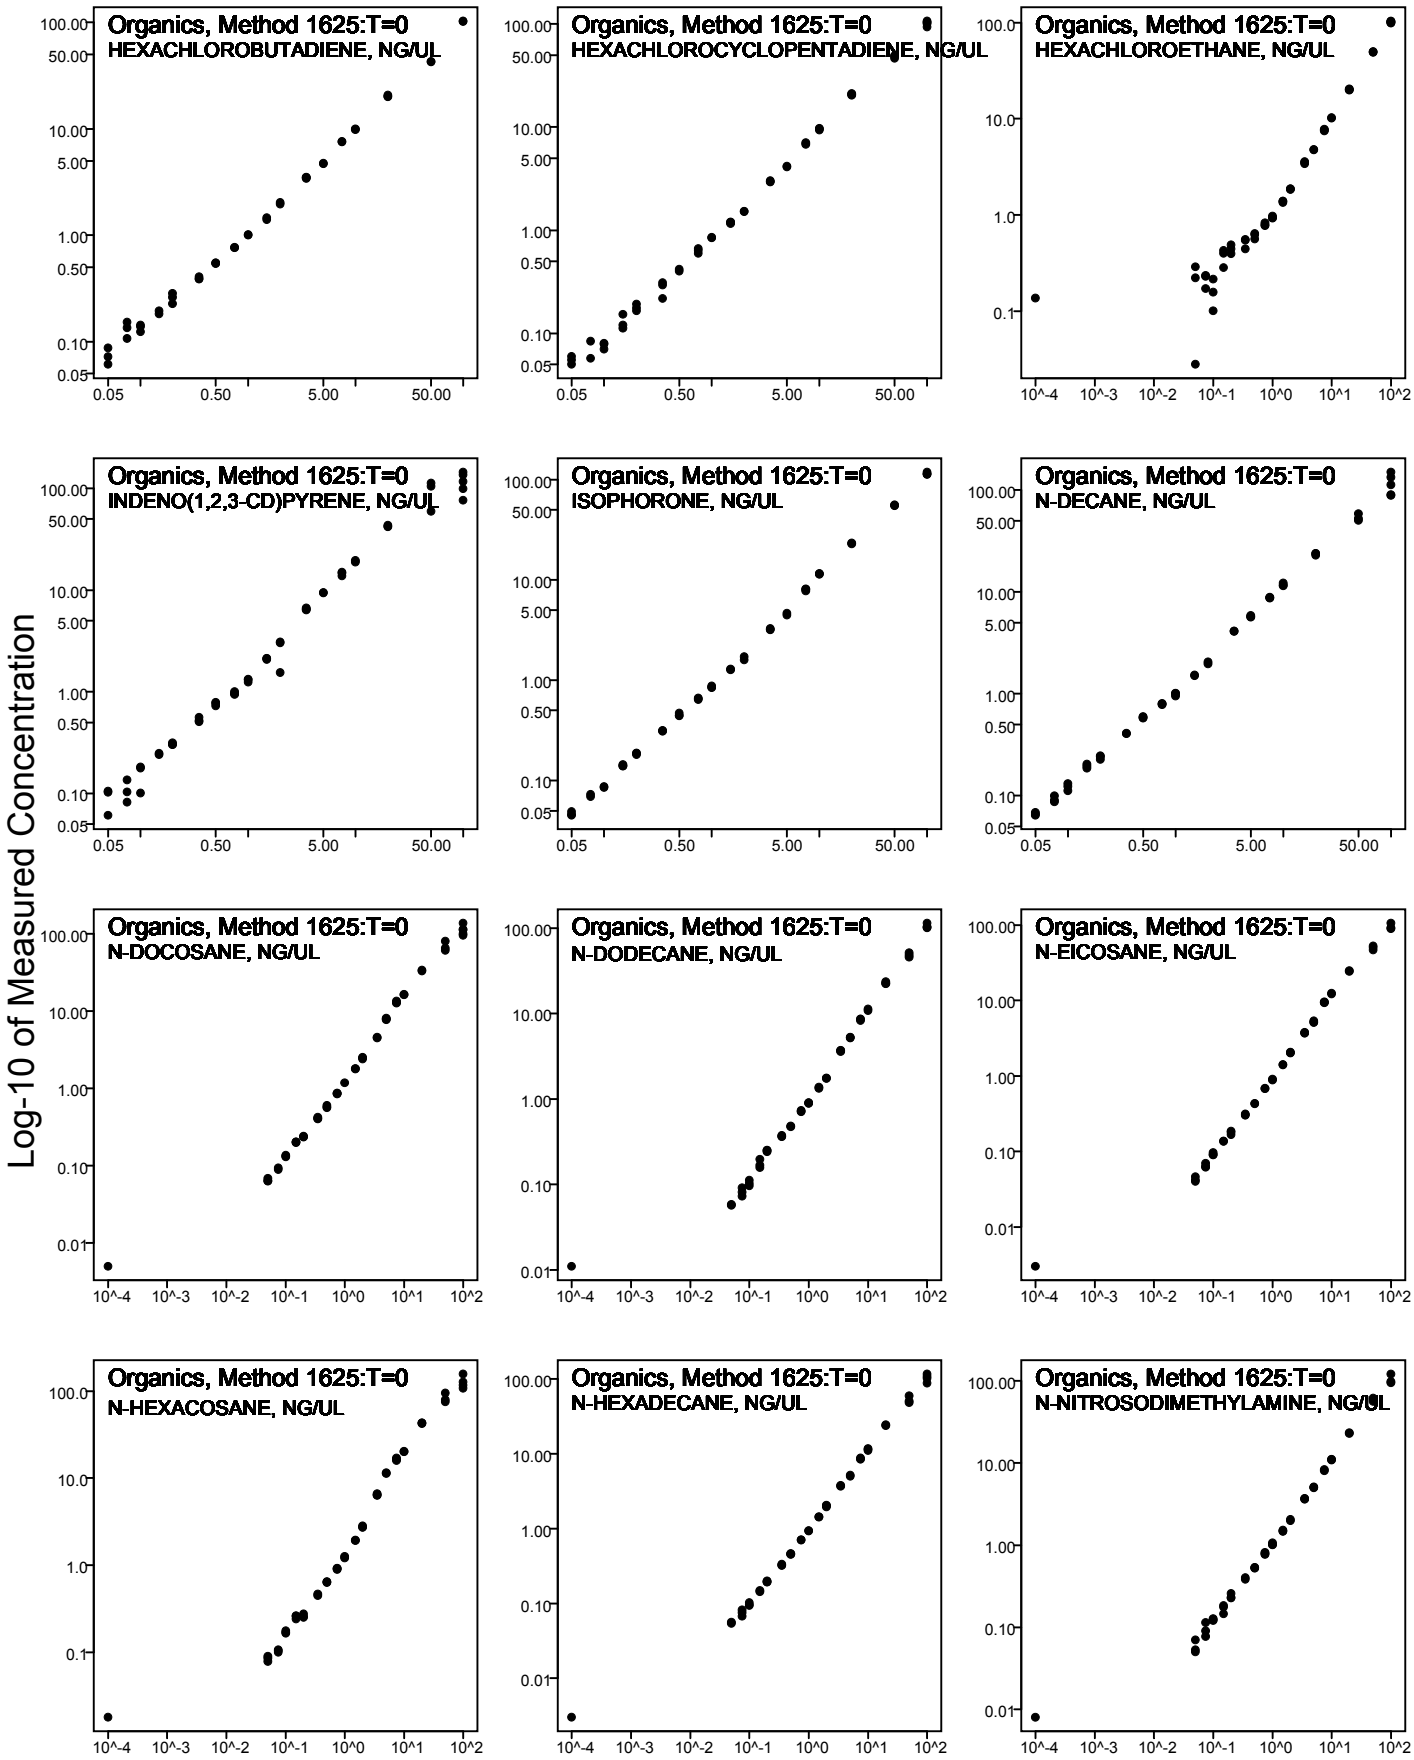

Measurement Results vs Spike Concentrations (Log-10 Scale)

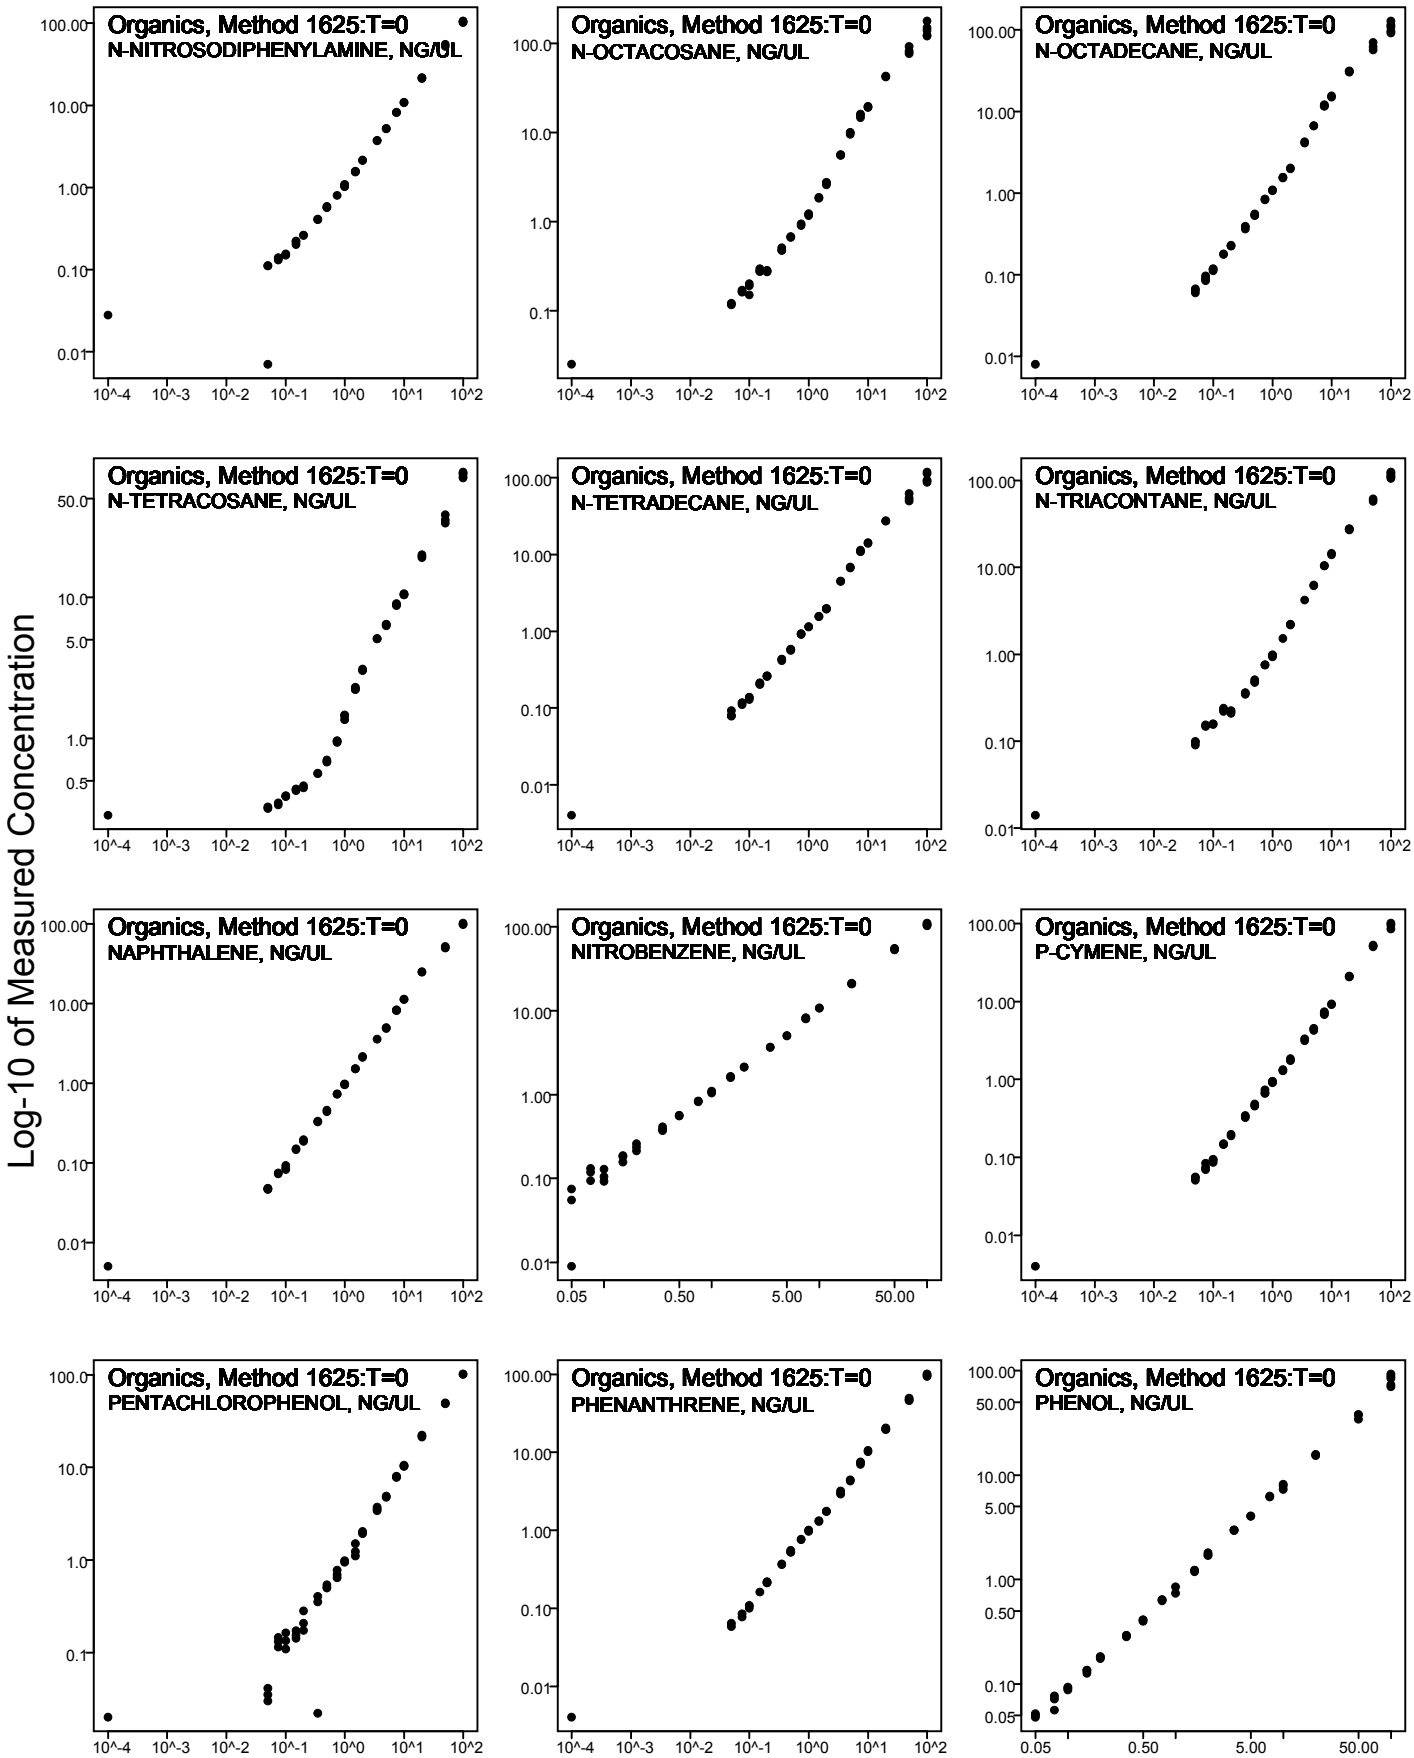

Measurement Results vs Spike Concentrations (Log-10 Scale)

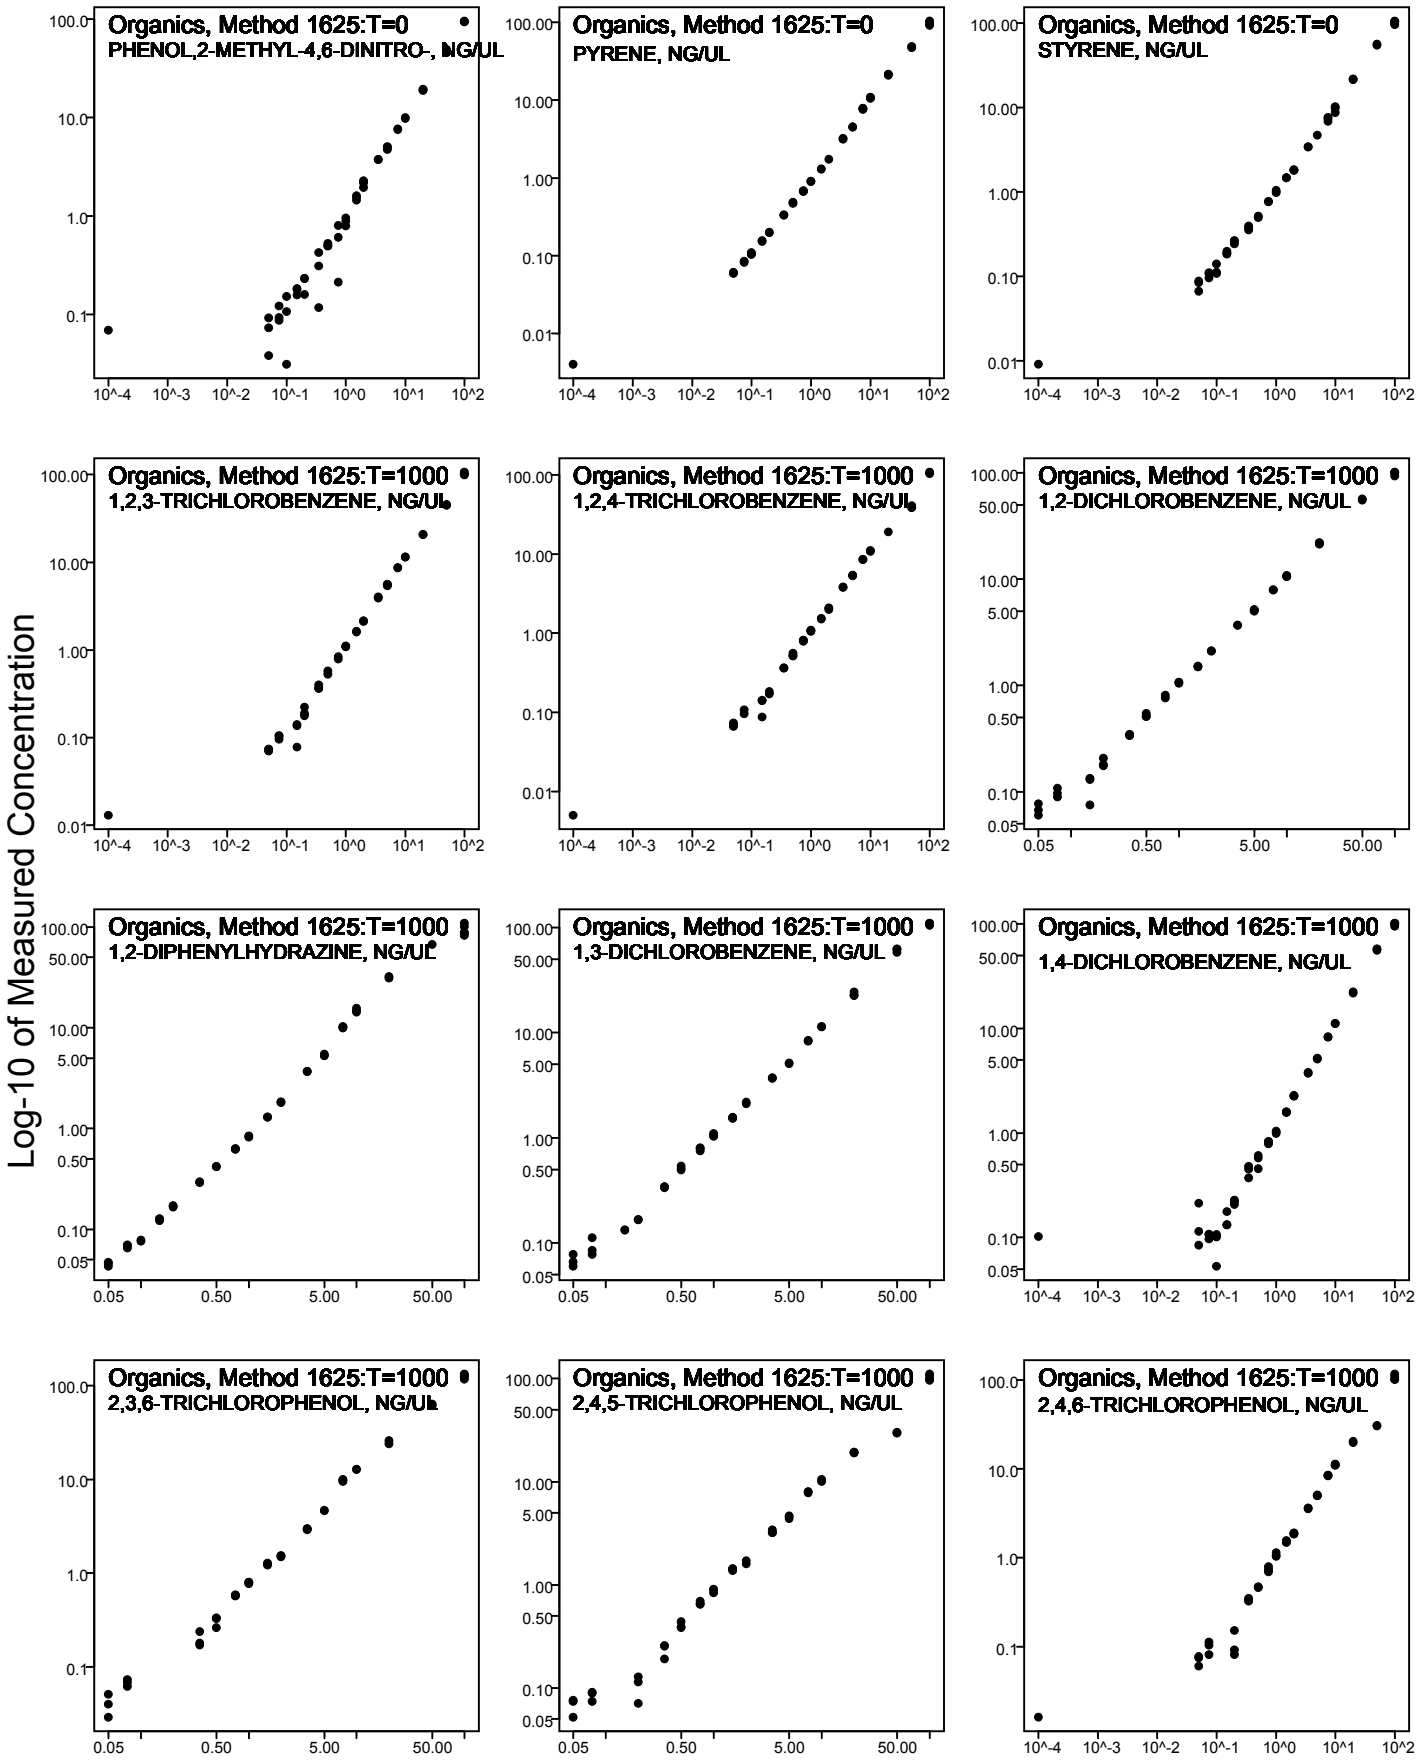

Measurement Results vs Spike Concentrations (Log-10 Scale)

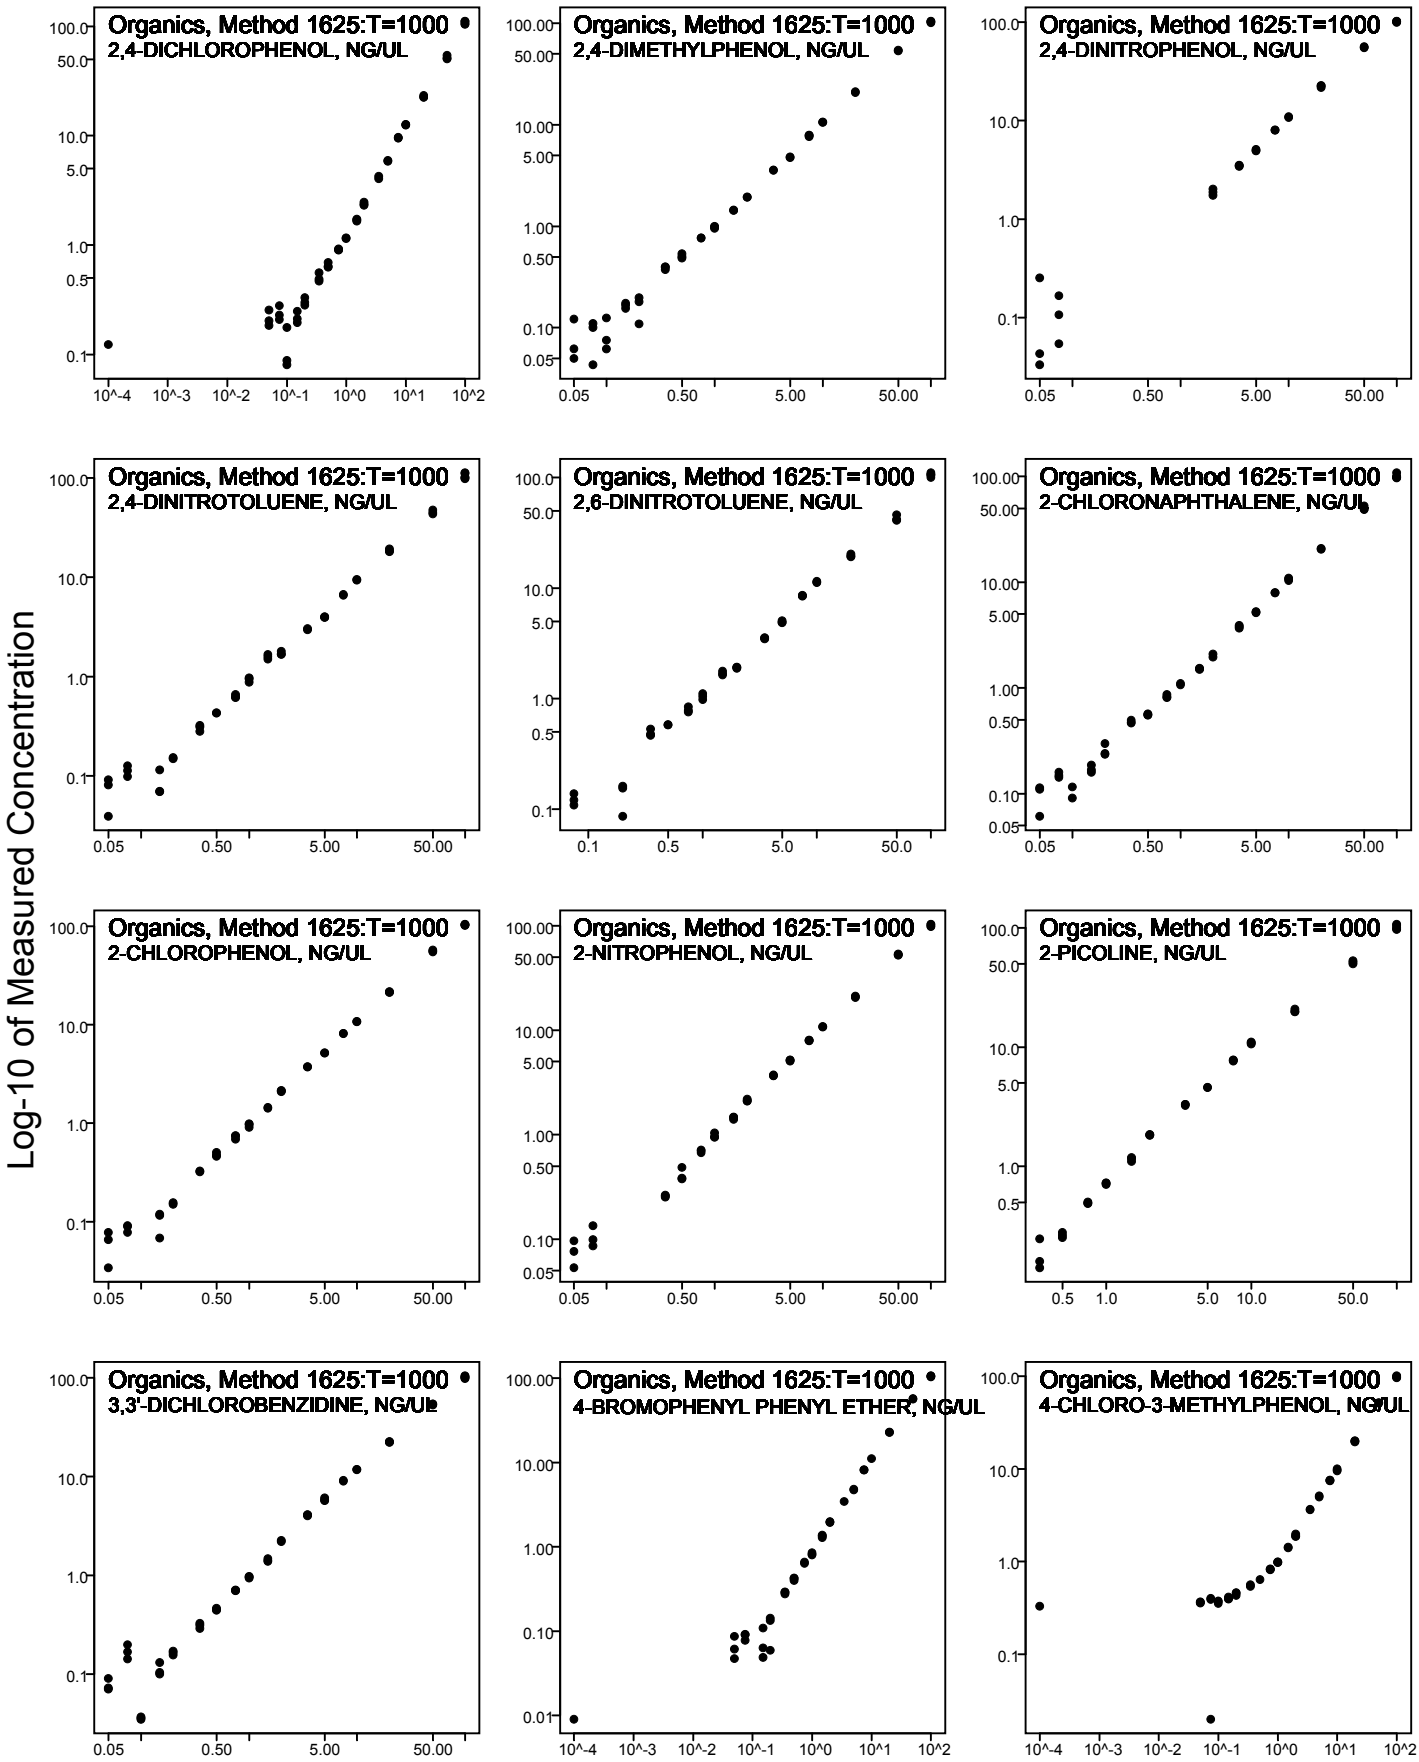

Measurement Results vs Spike Concentrations (Log-10 Scale)

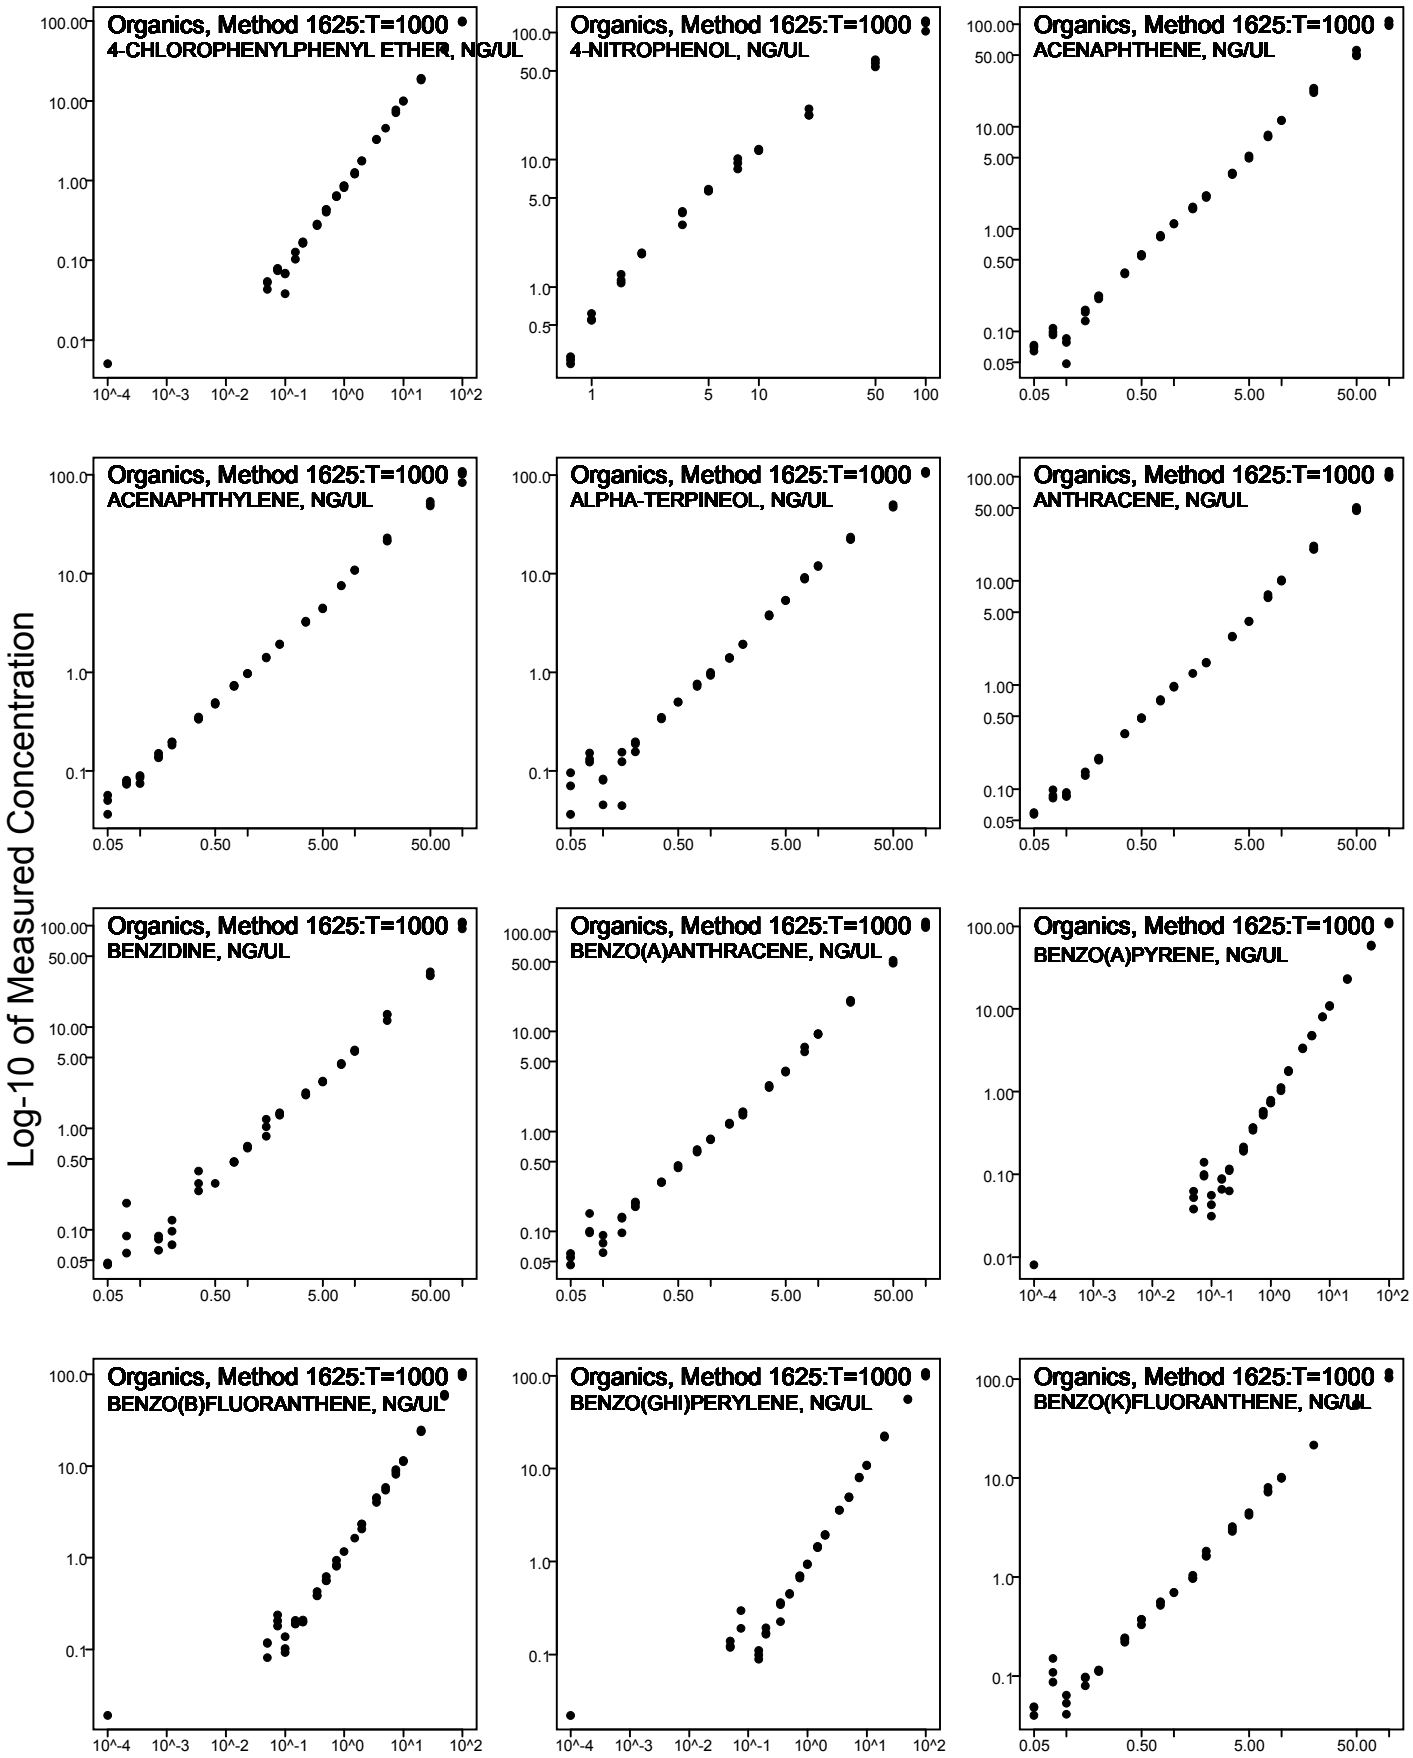

Measurement Results vs Spike Concentrations (Log-10 Scale)

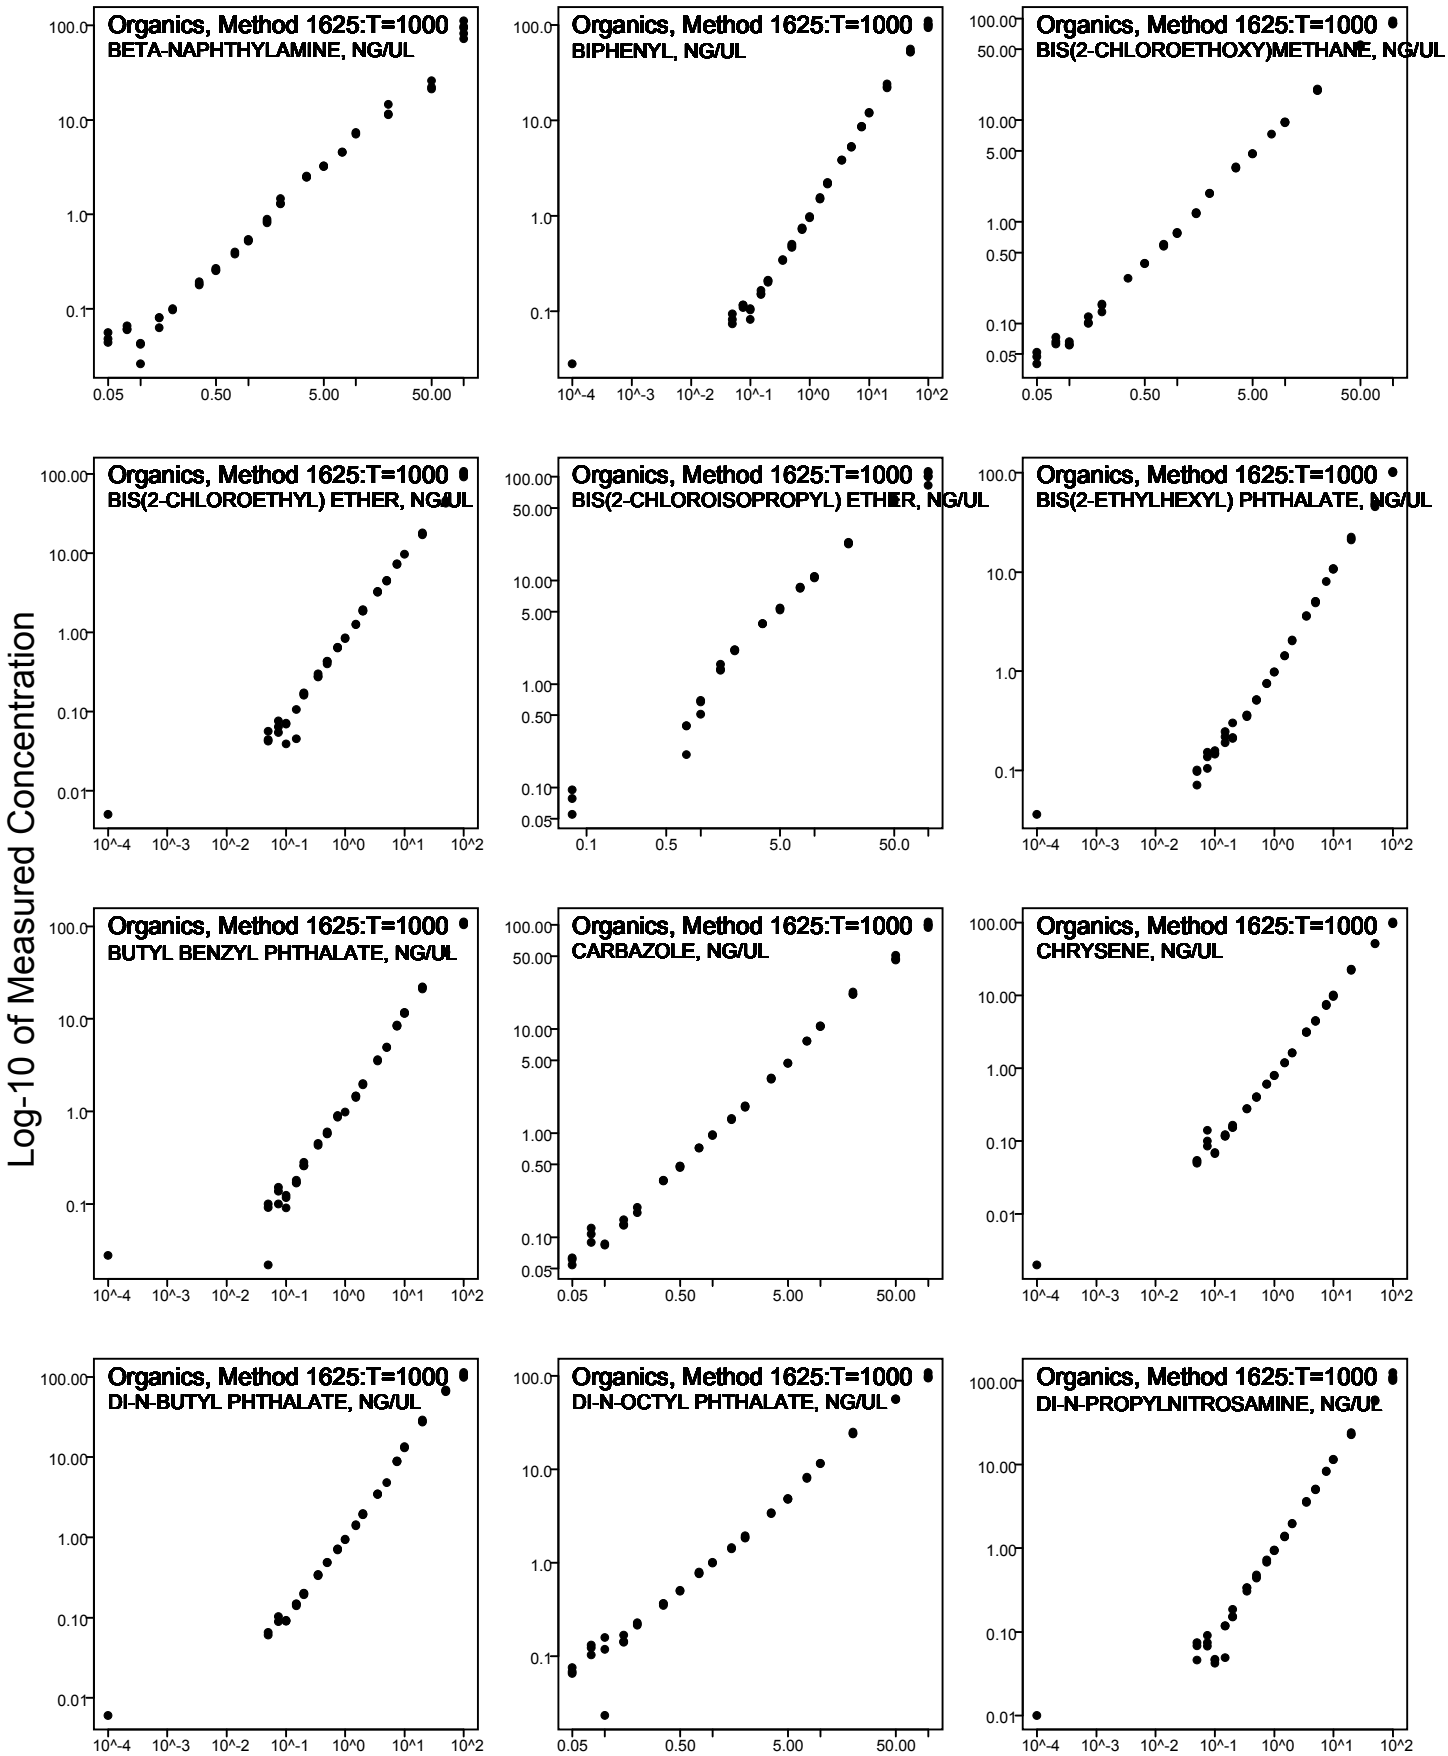

Measurement Results vs Spike Concentrations (Log-10 Scale)

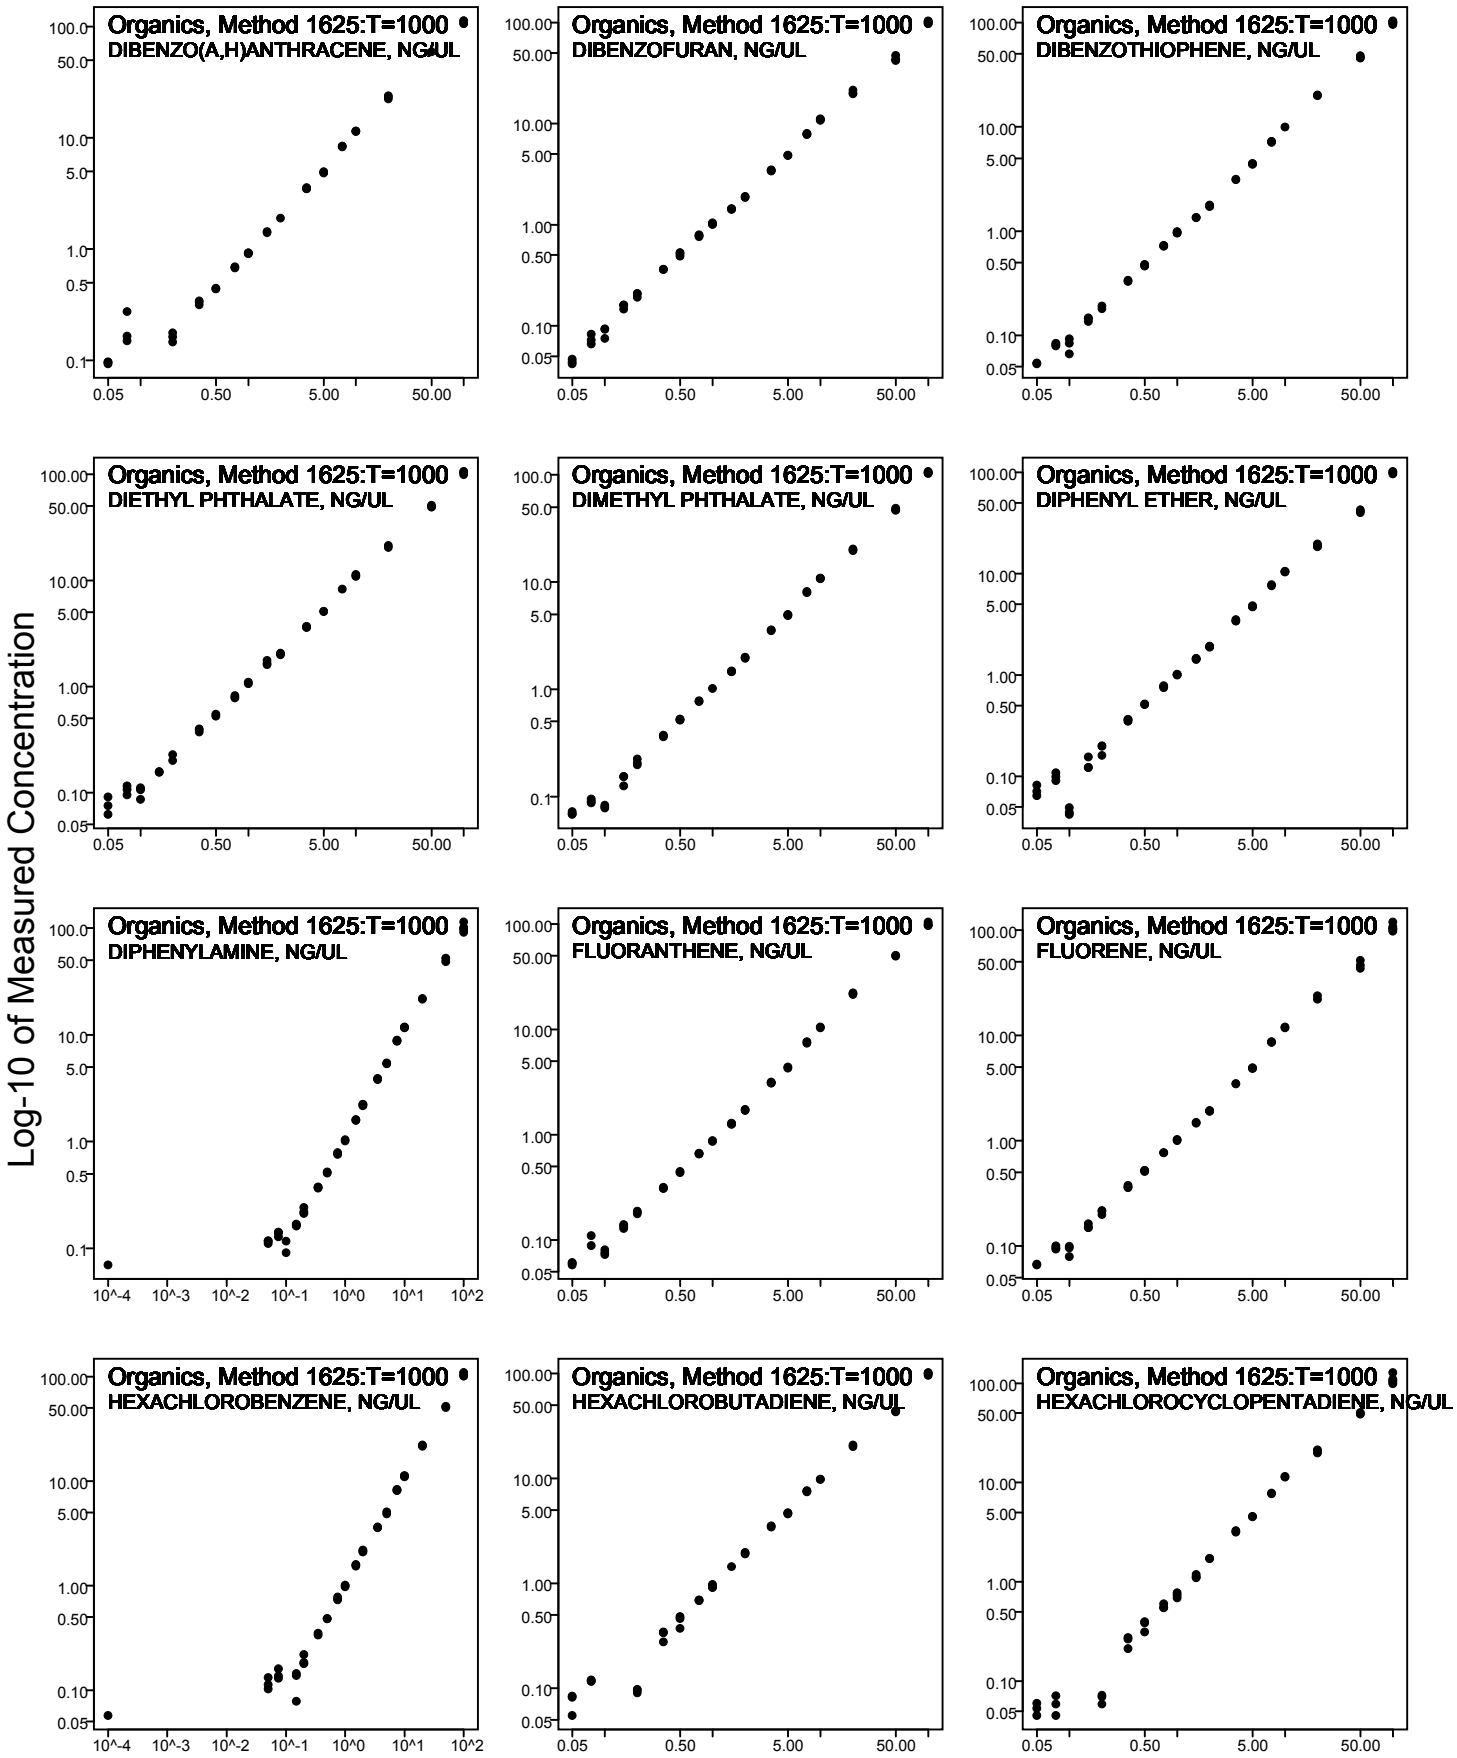

Measurement Results vs Spike Concentrations (Log-10 Scale)

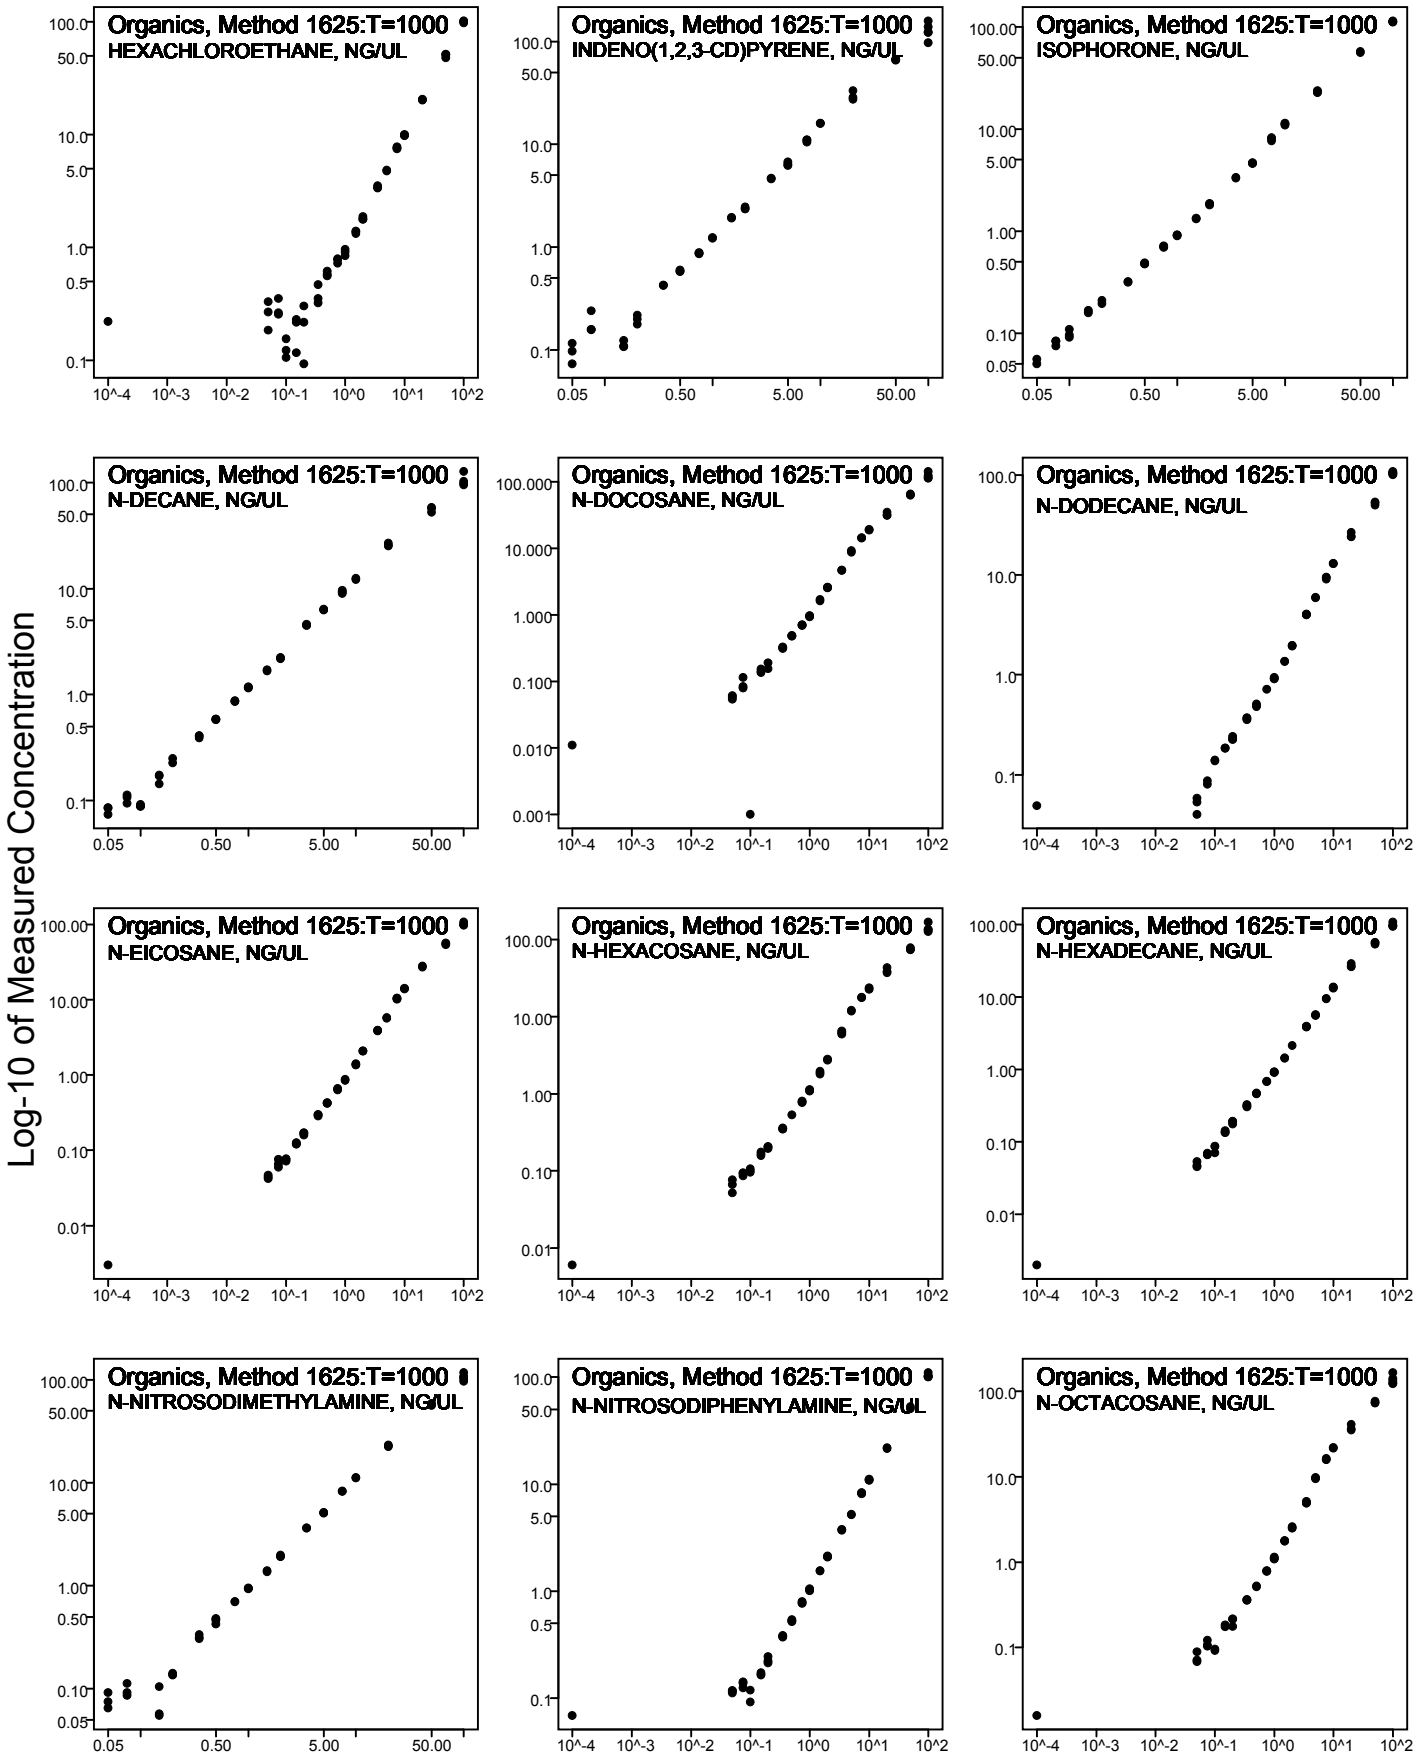

Measurement Results vs Spike Concentrations (Log-10 Scale)

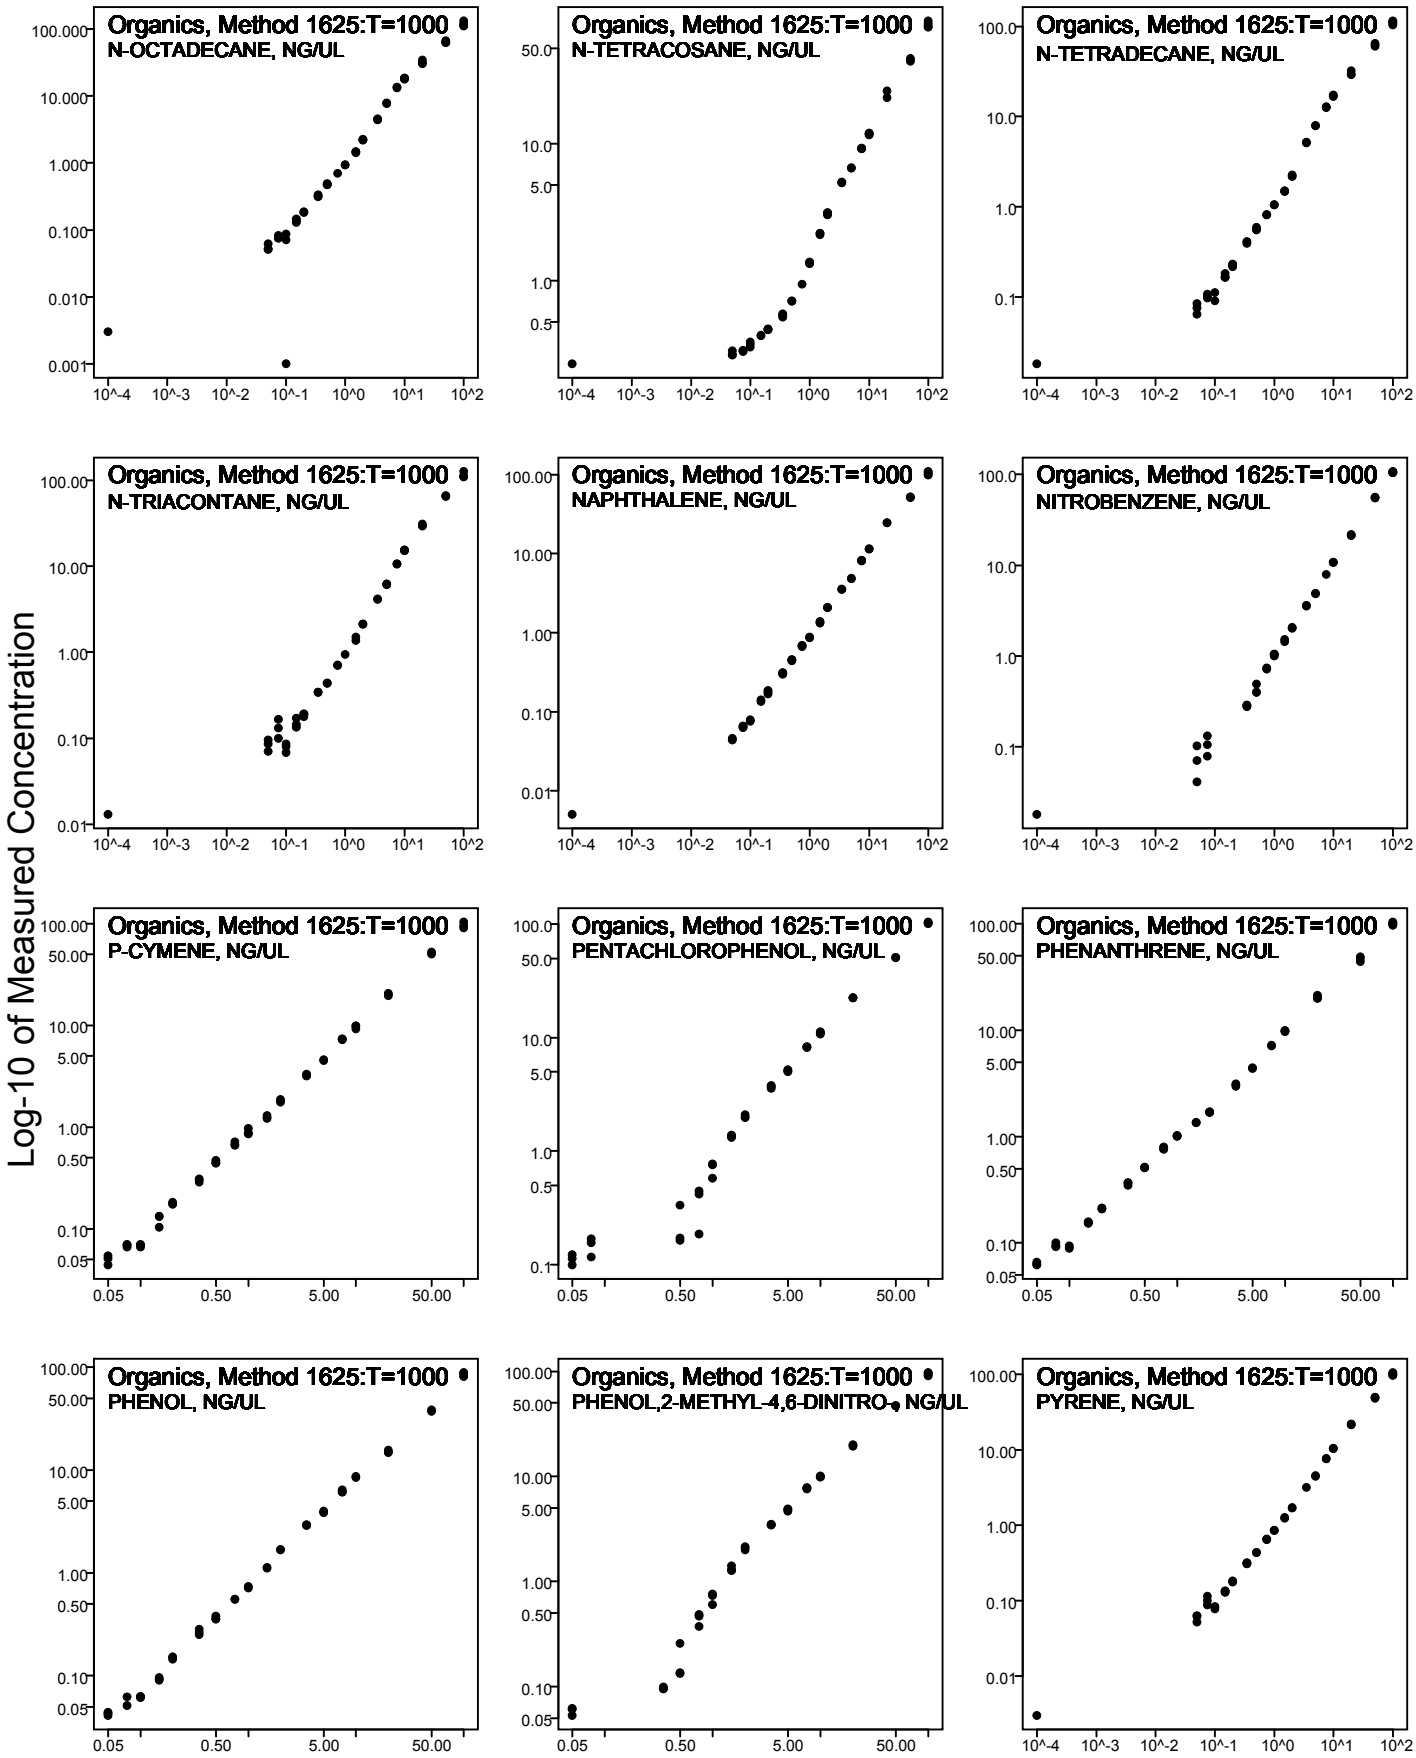

Measurement Results vs Spike Concentrations (Log-10 Scale)

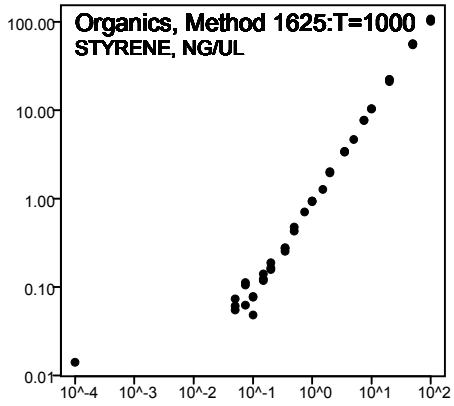

Log-10 of Measured Concentration

Log-10 of Spike Concentration

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

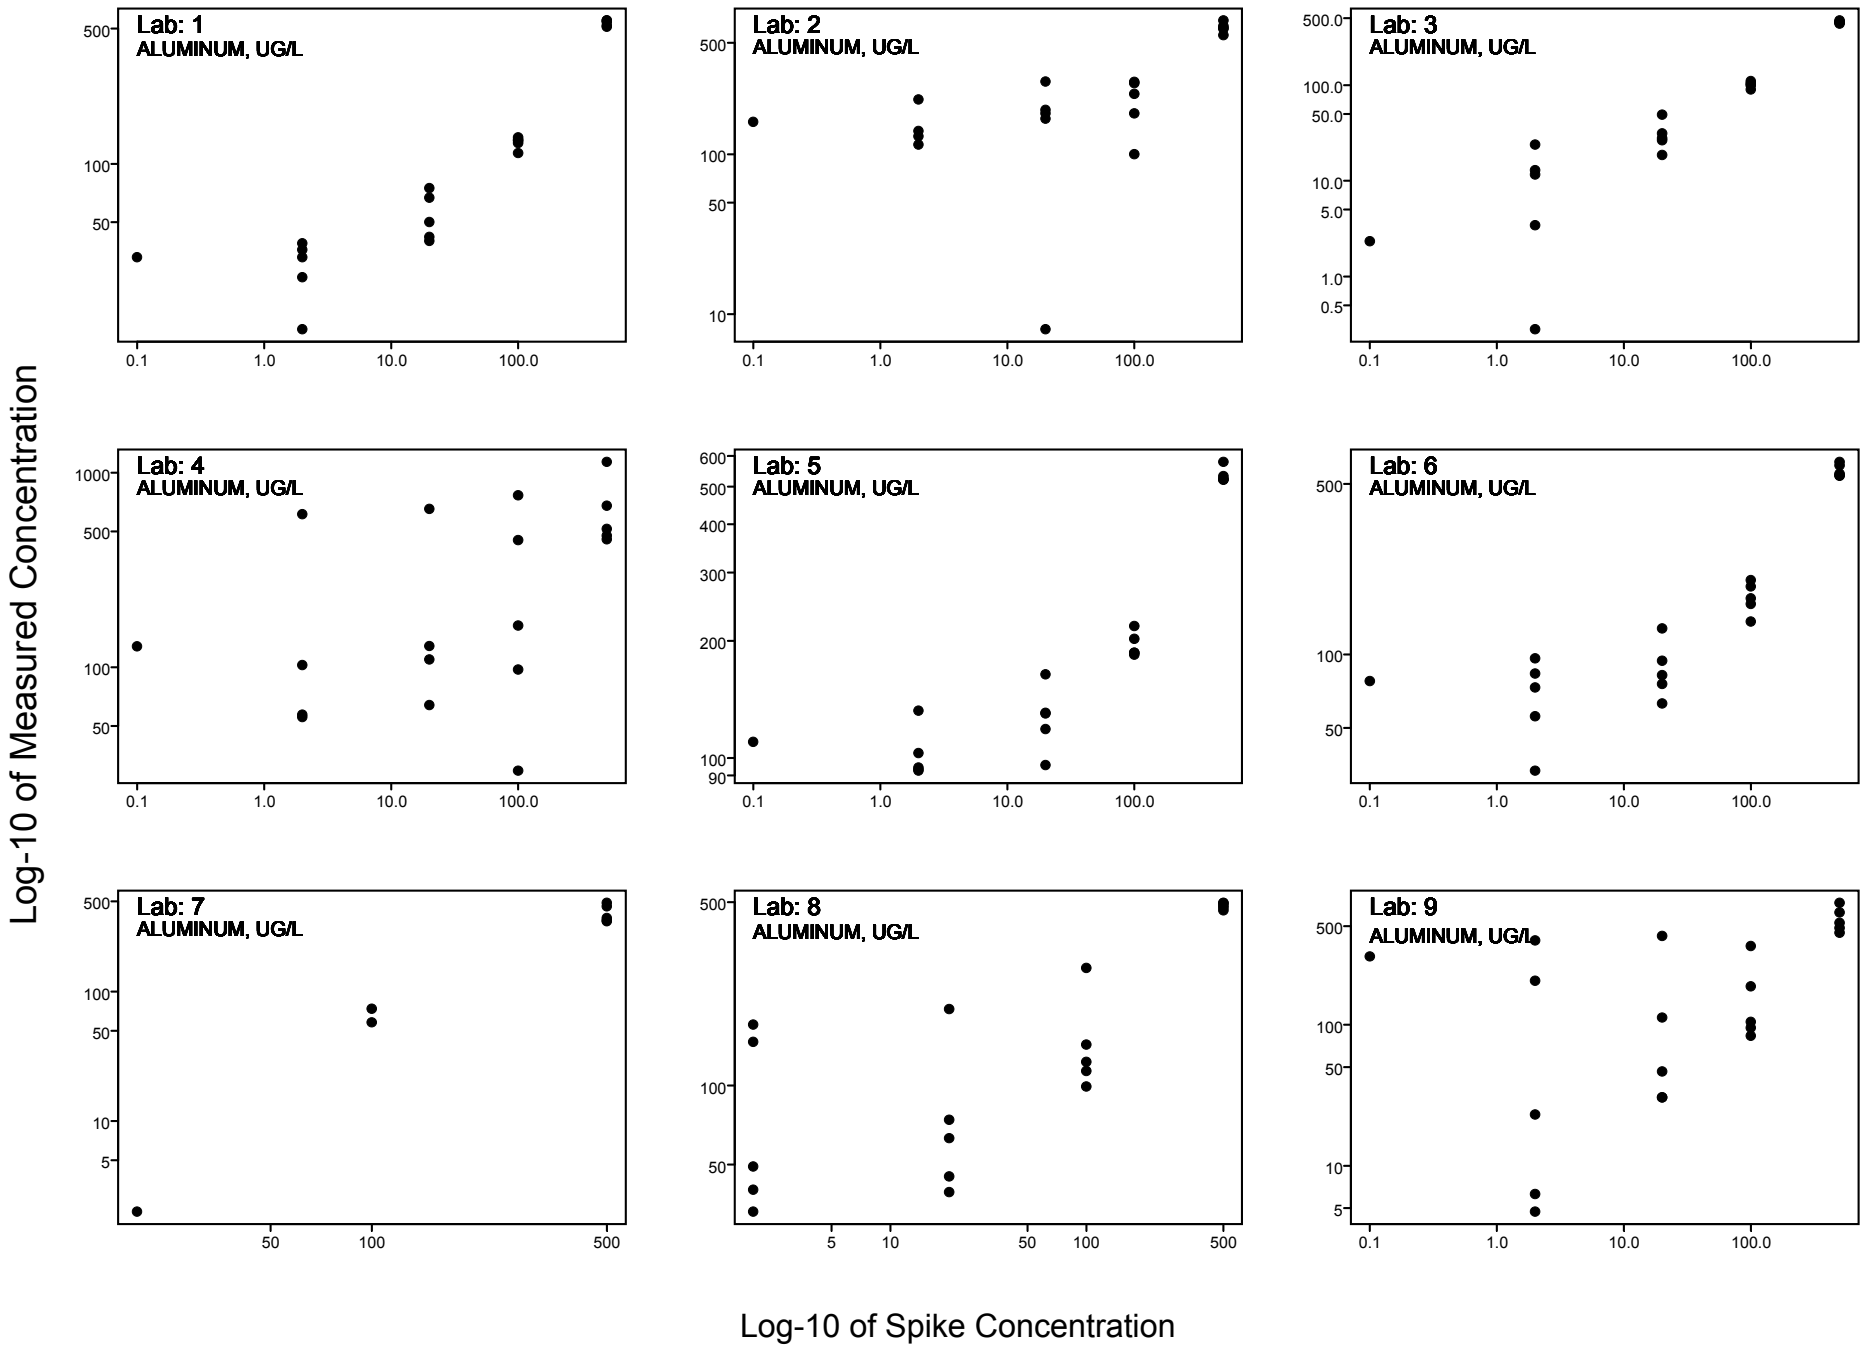

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

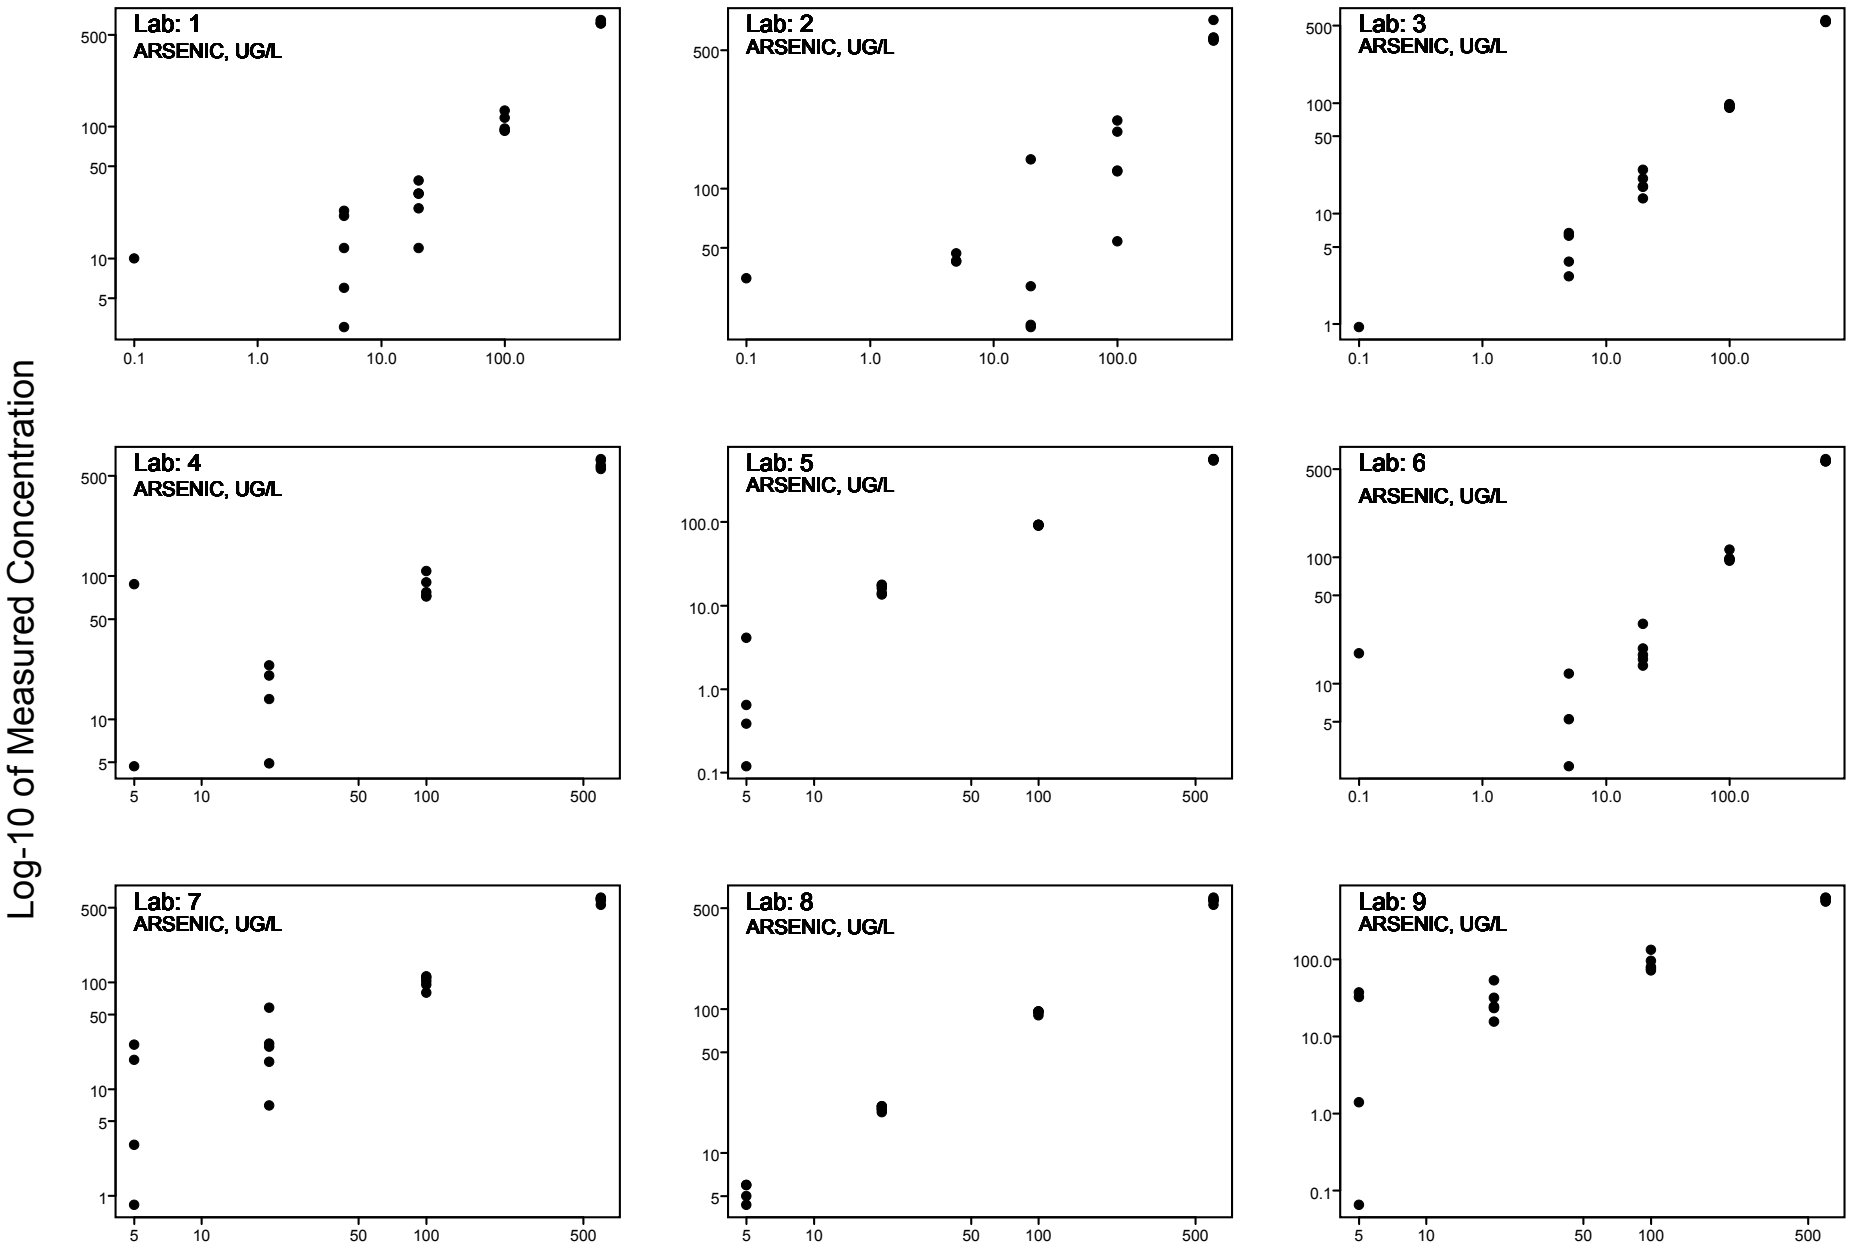

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

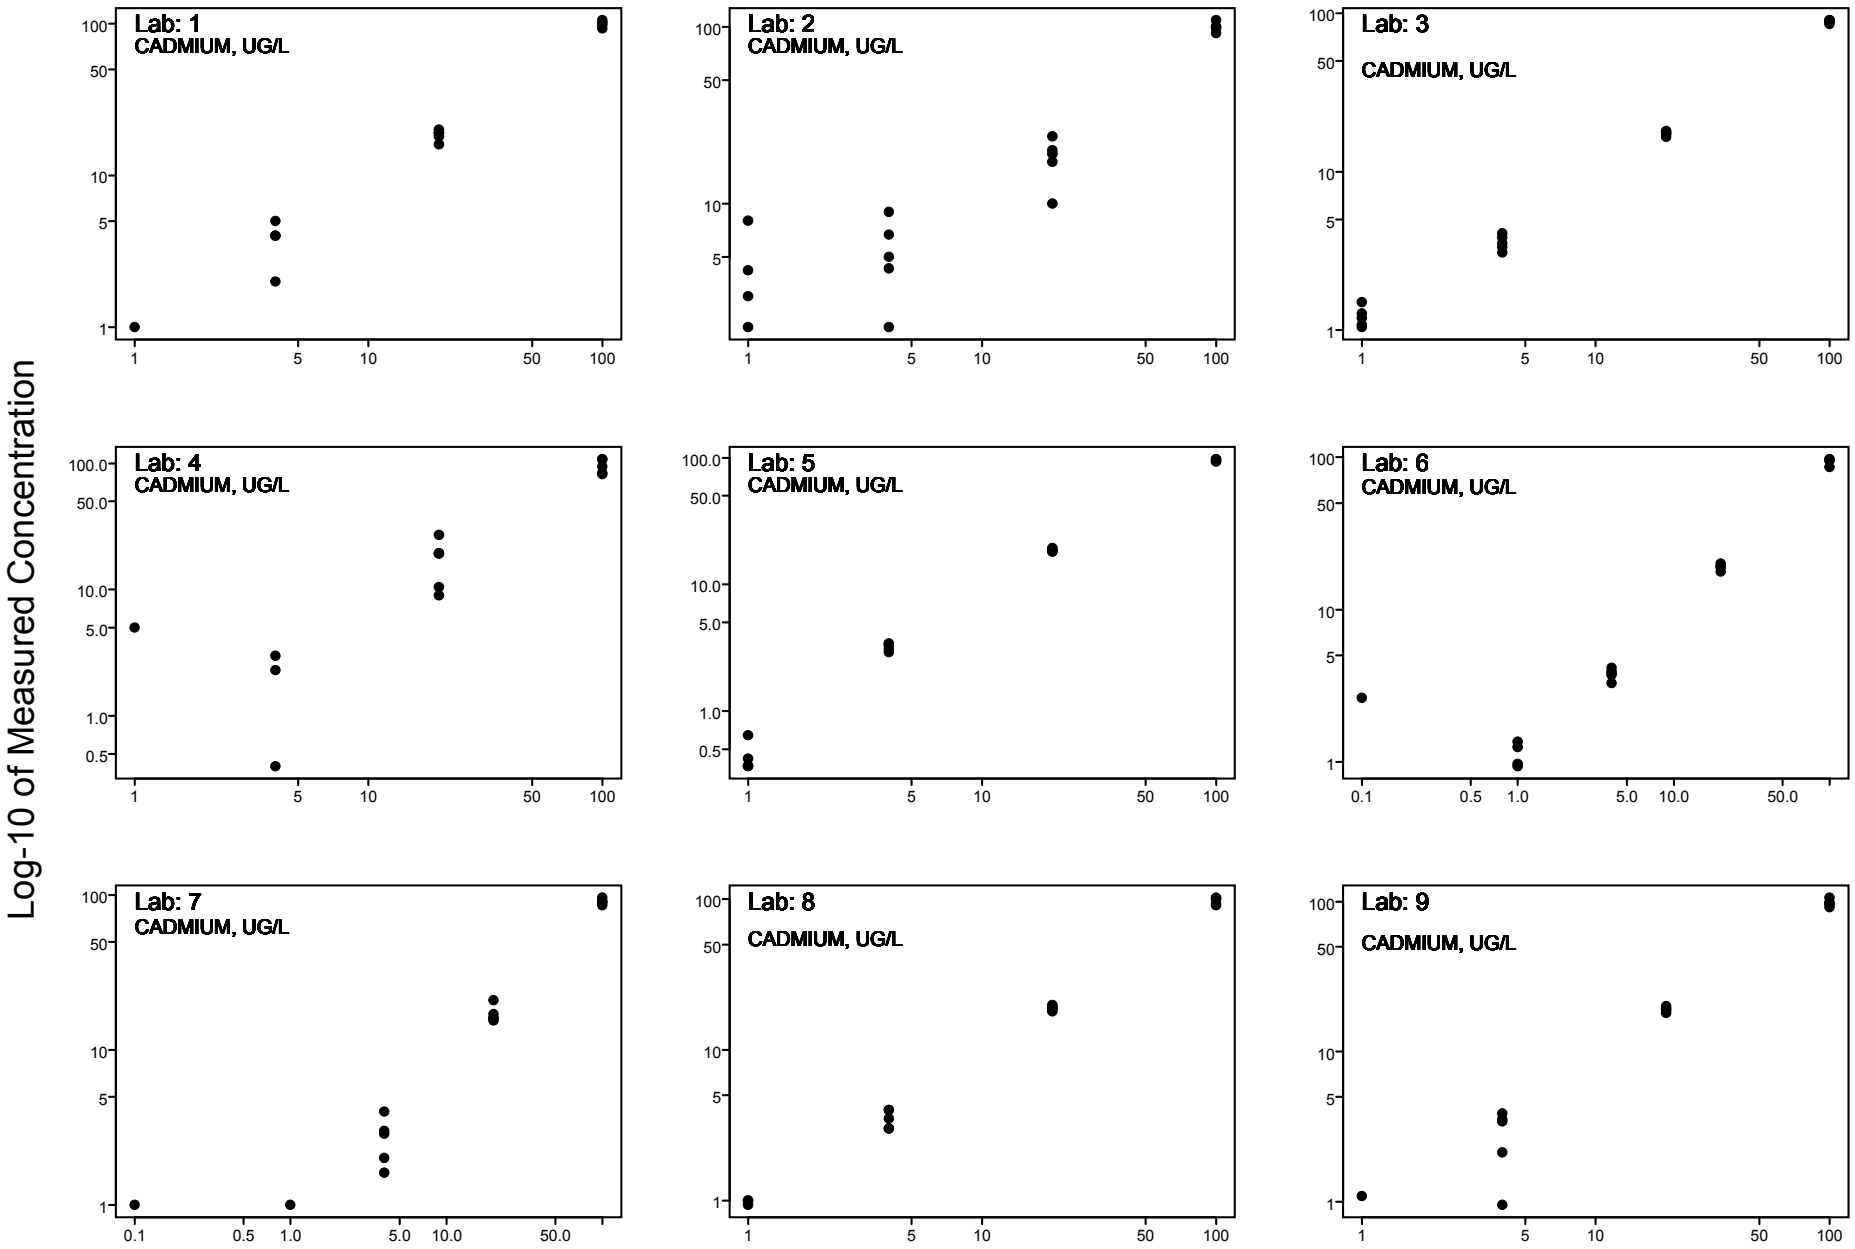

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

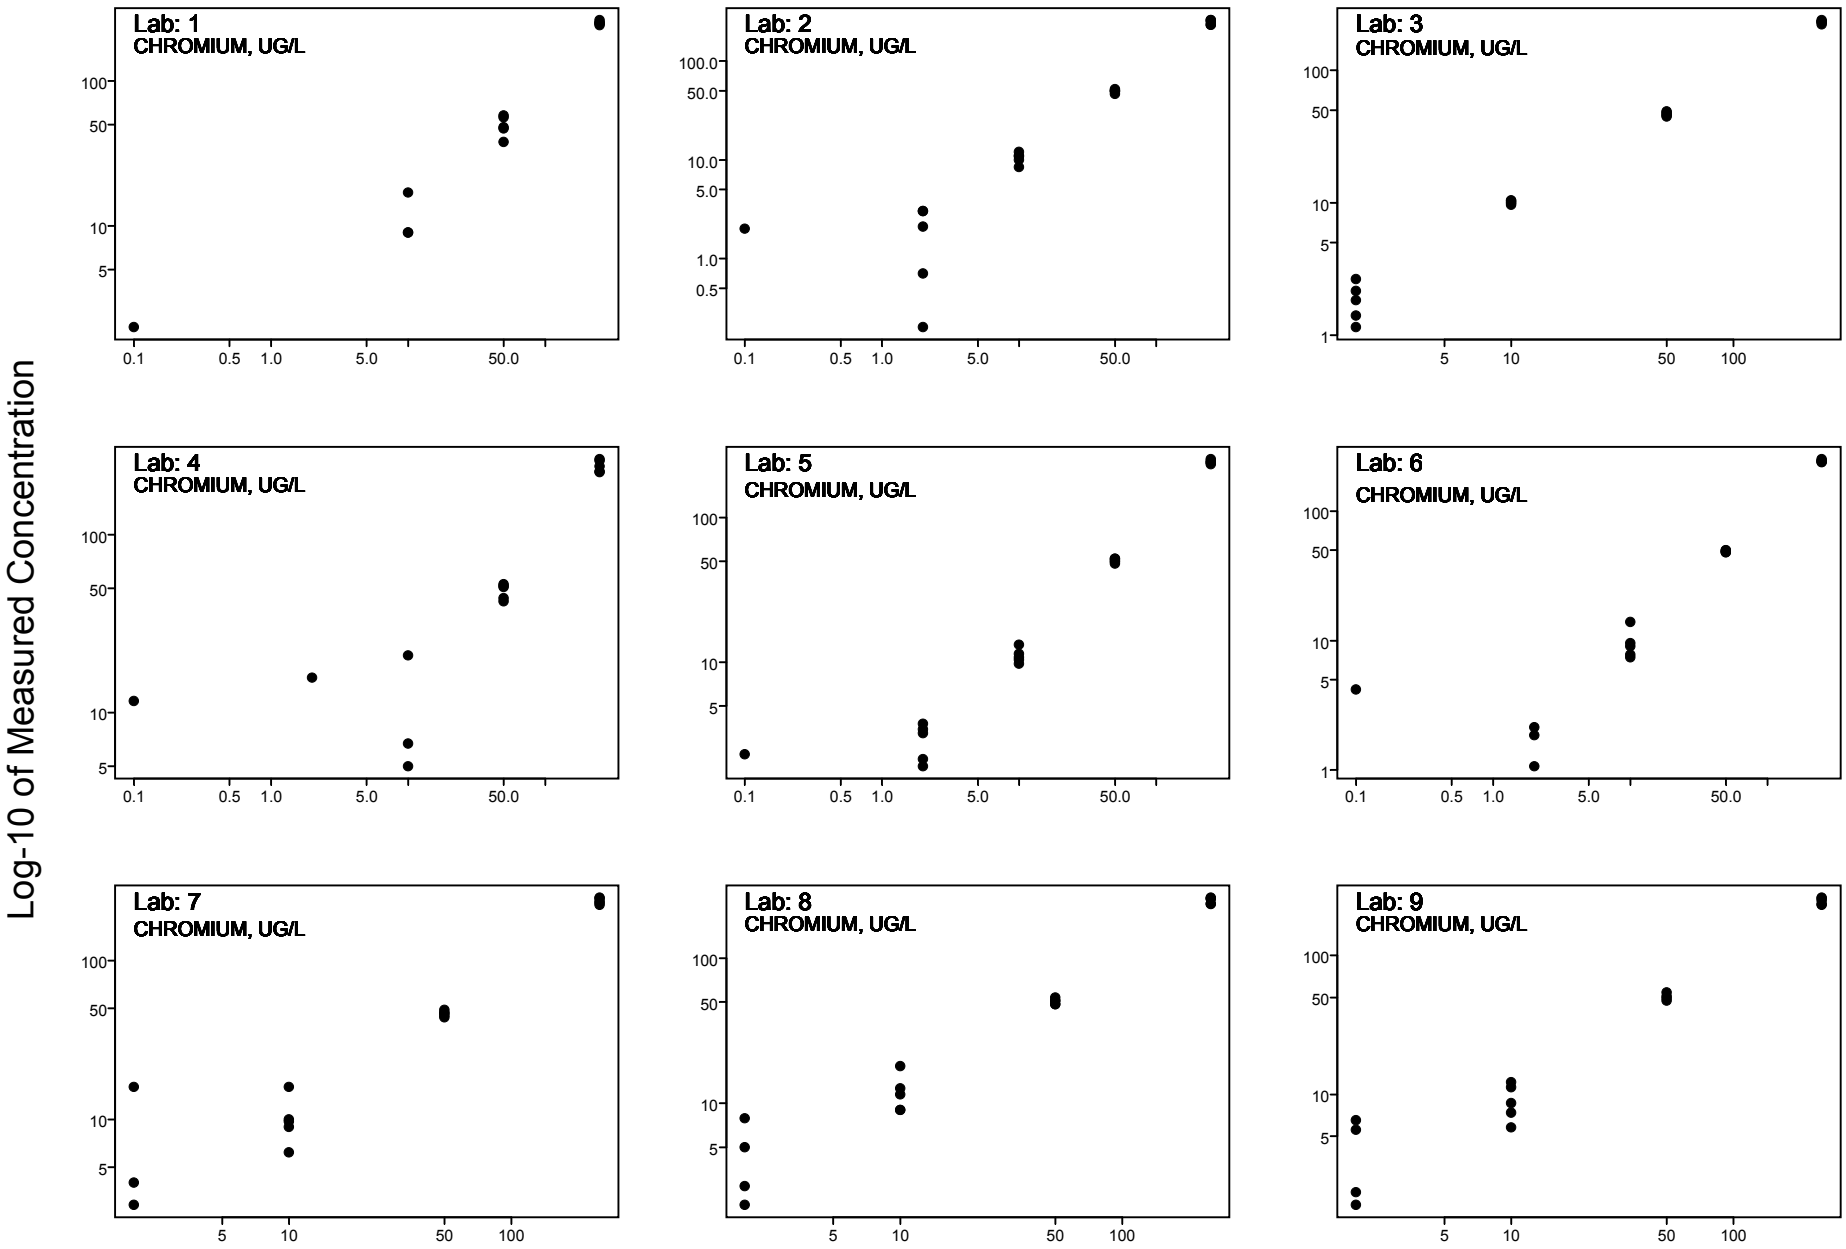

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

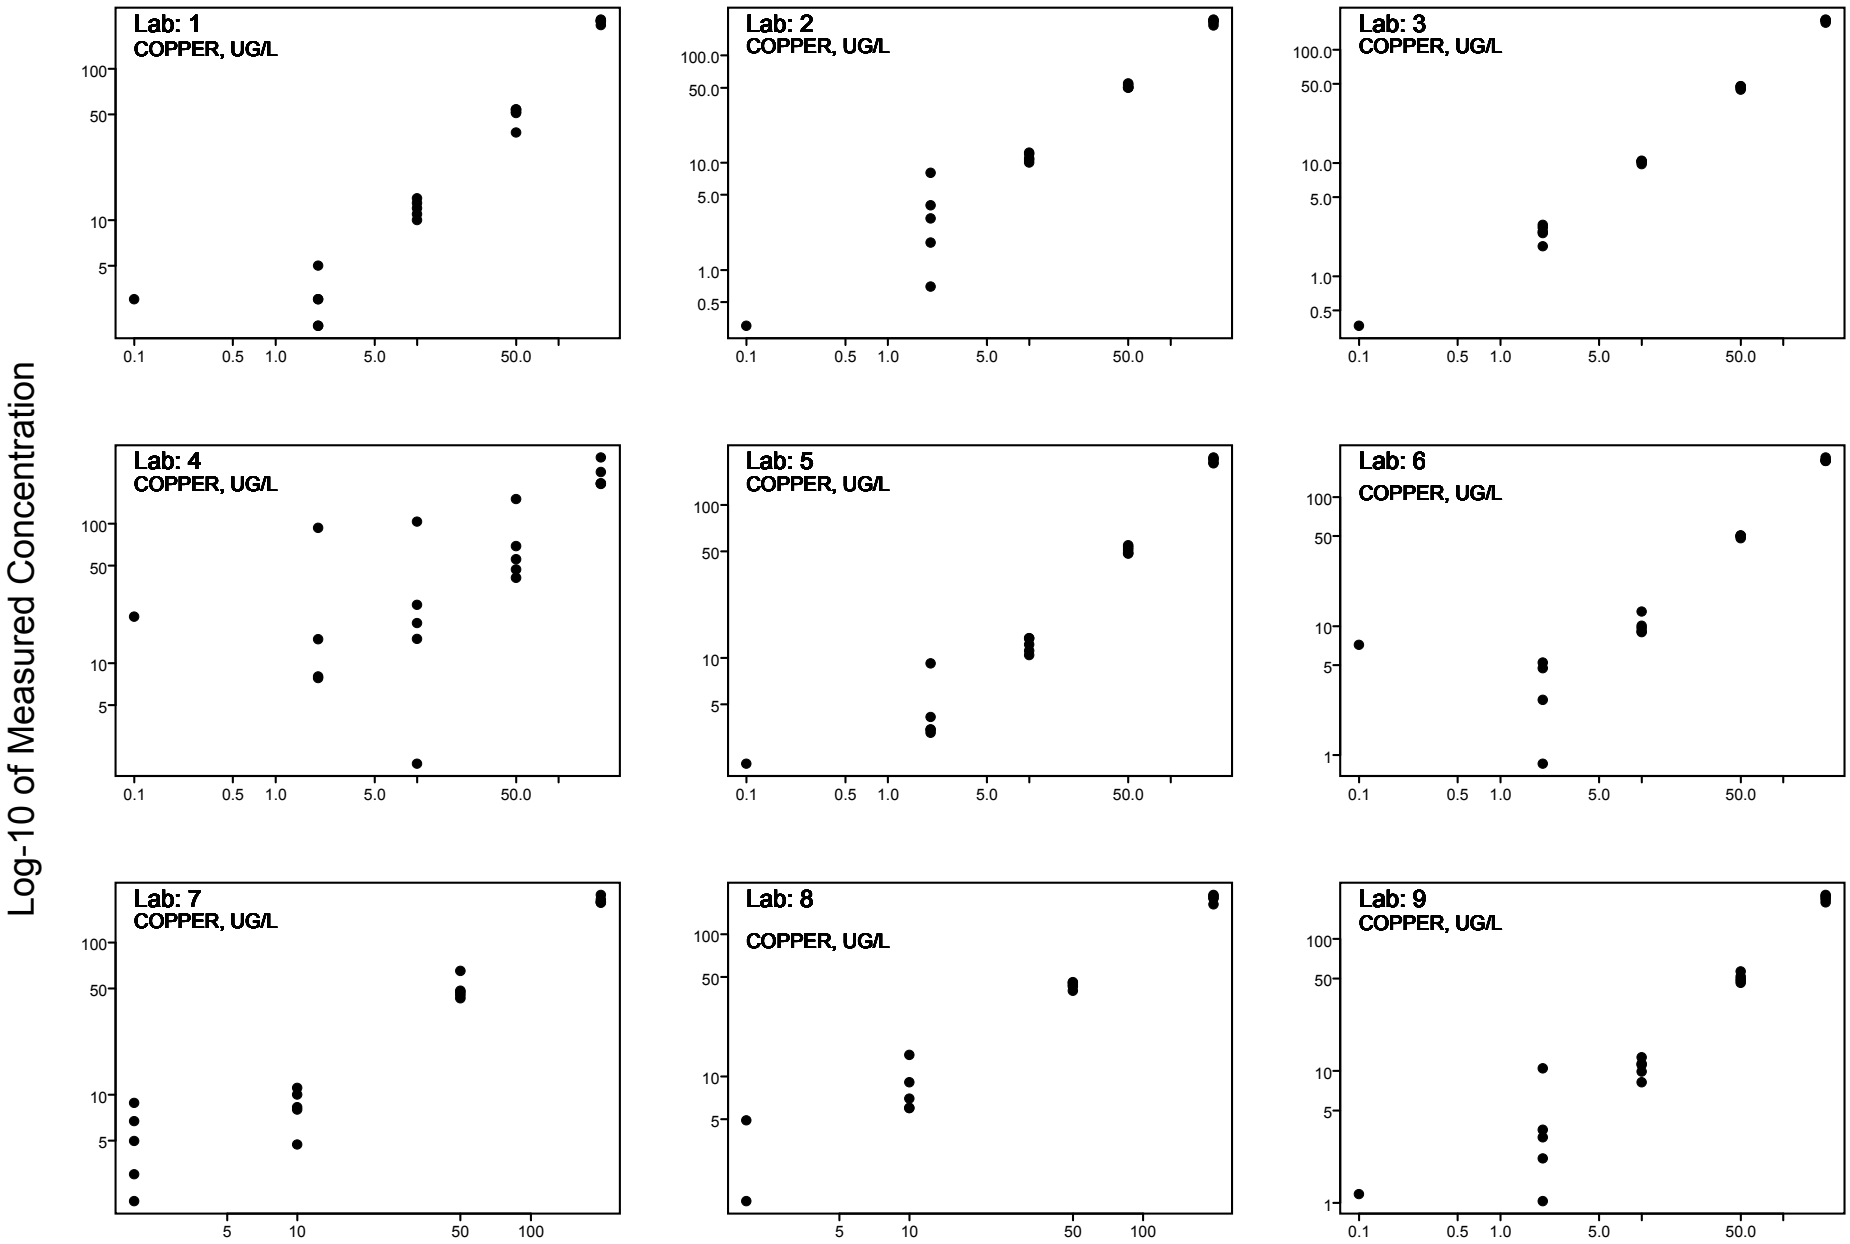

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

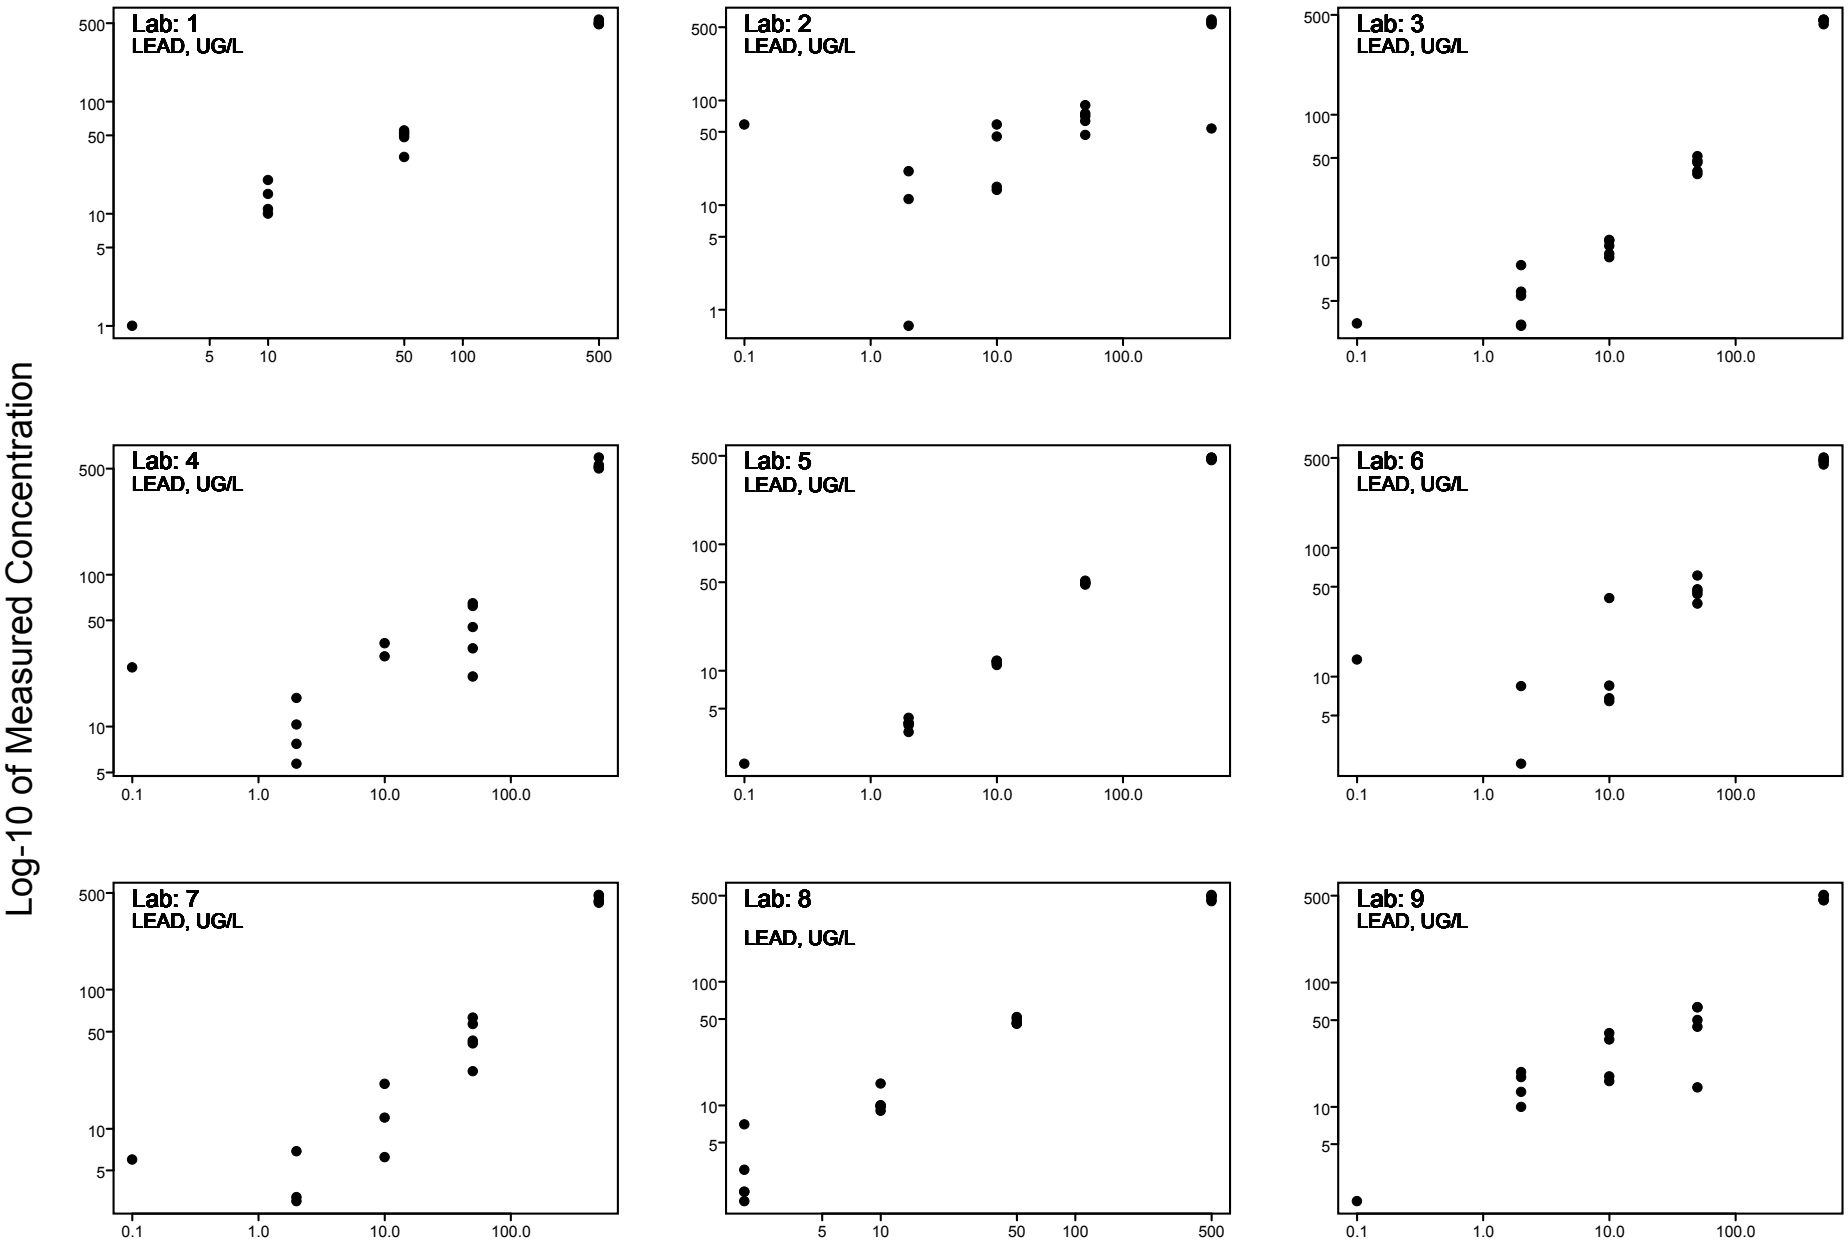

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

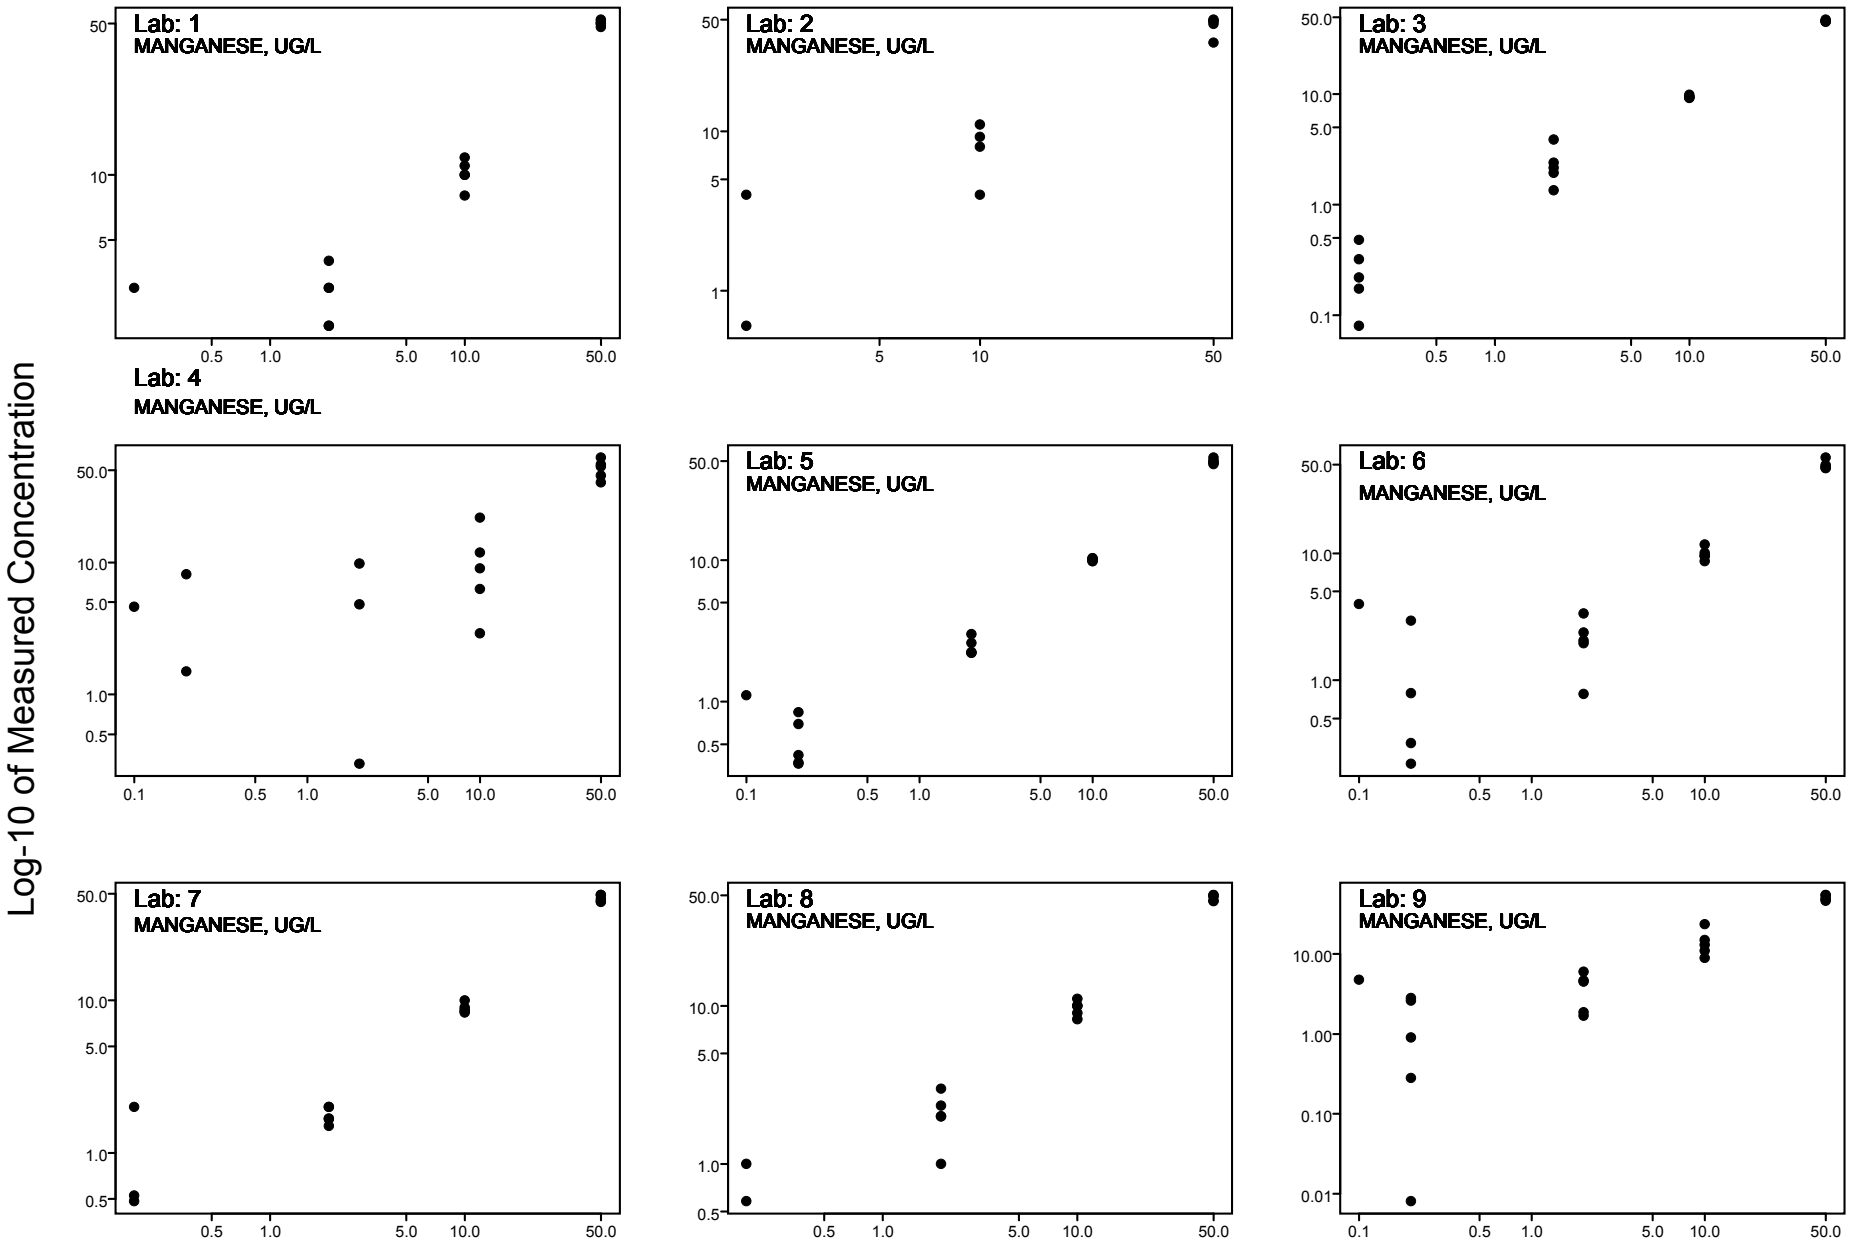

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 245 CVA)

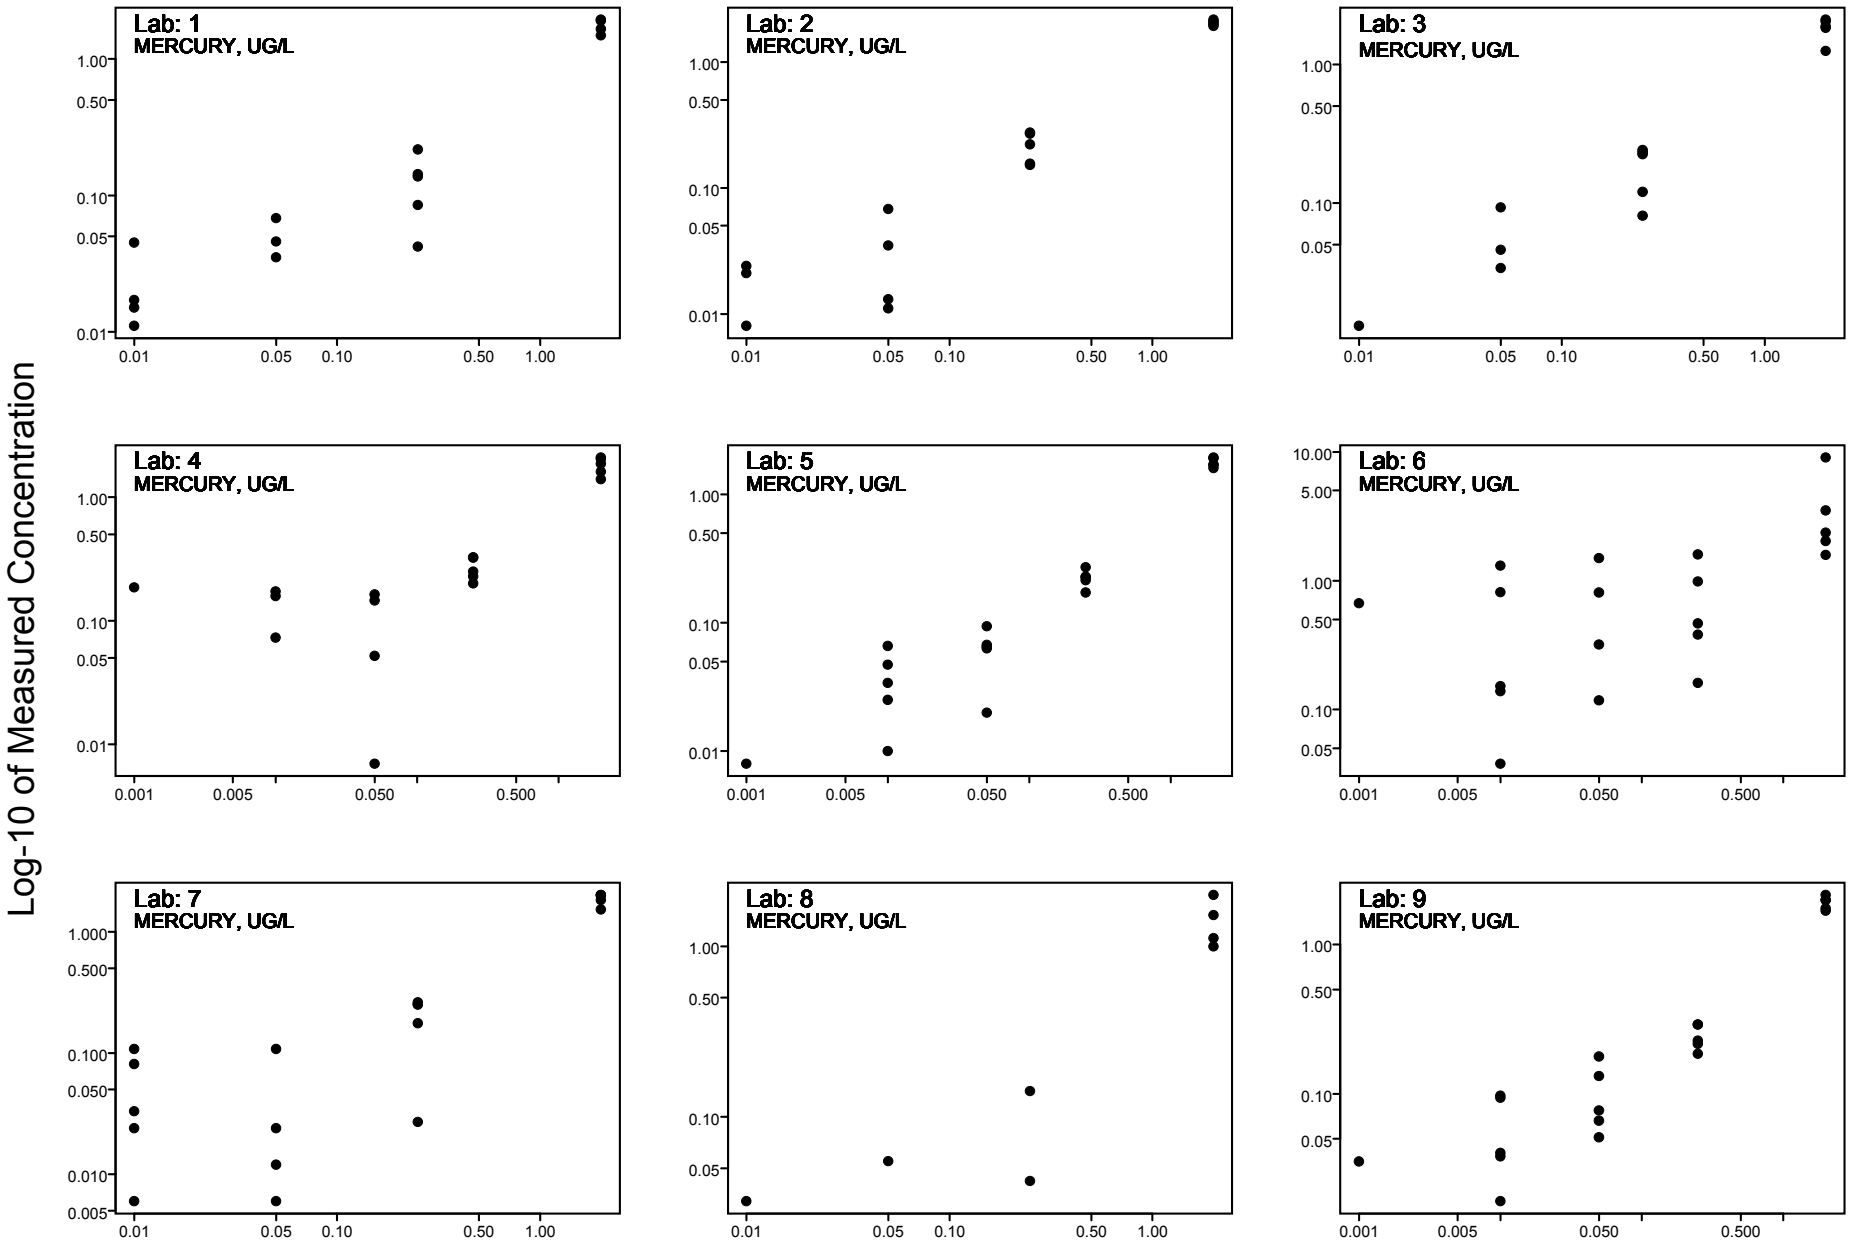

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

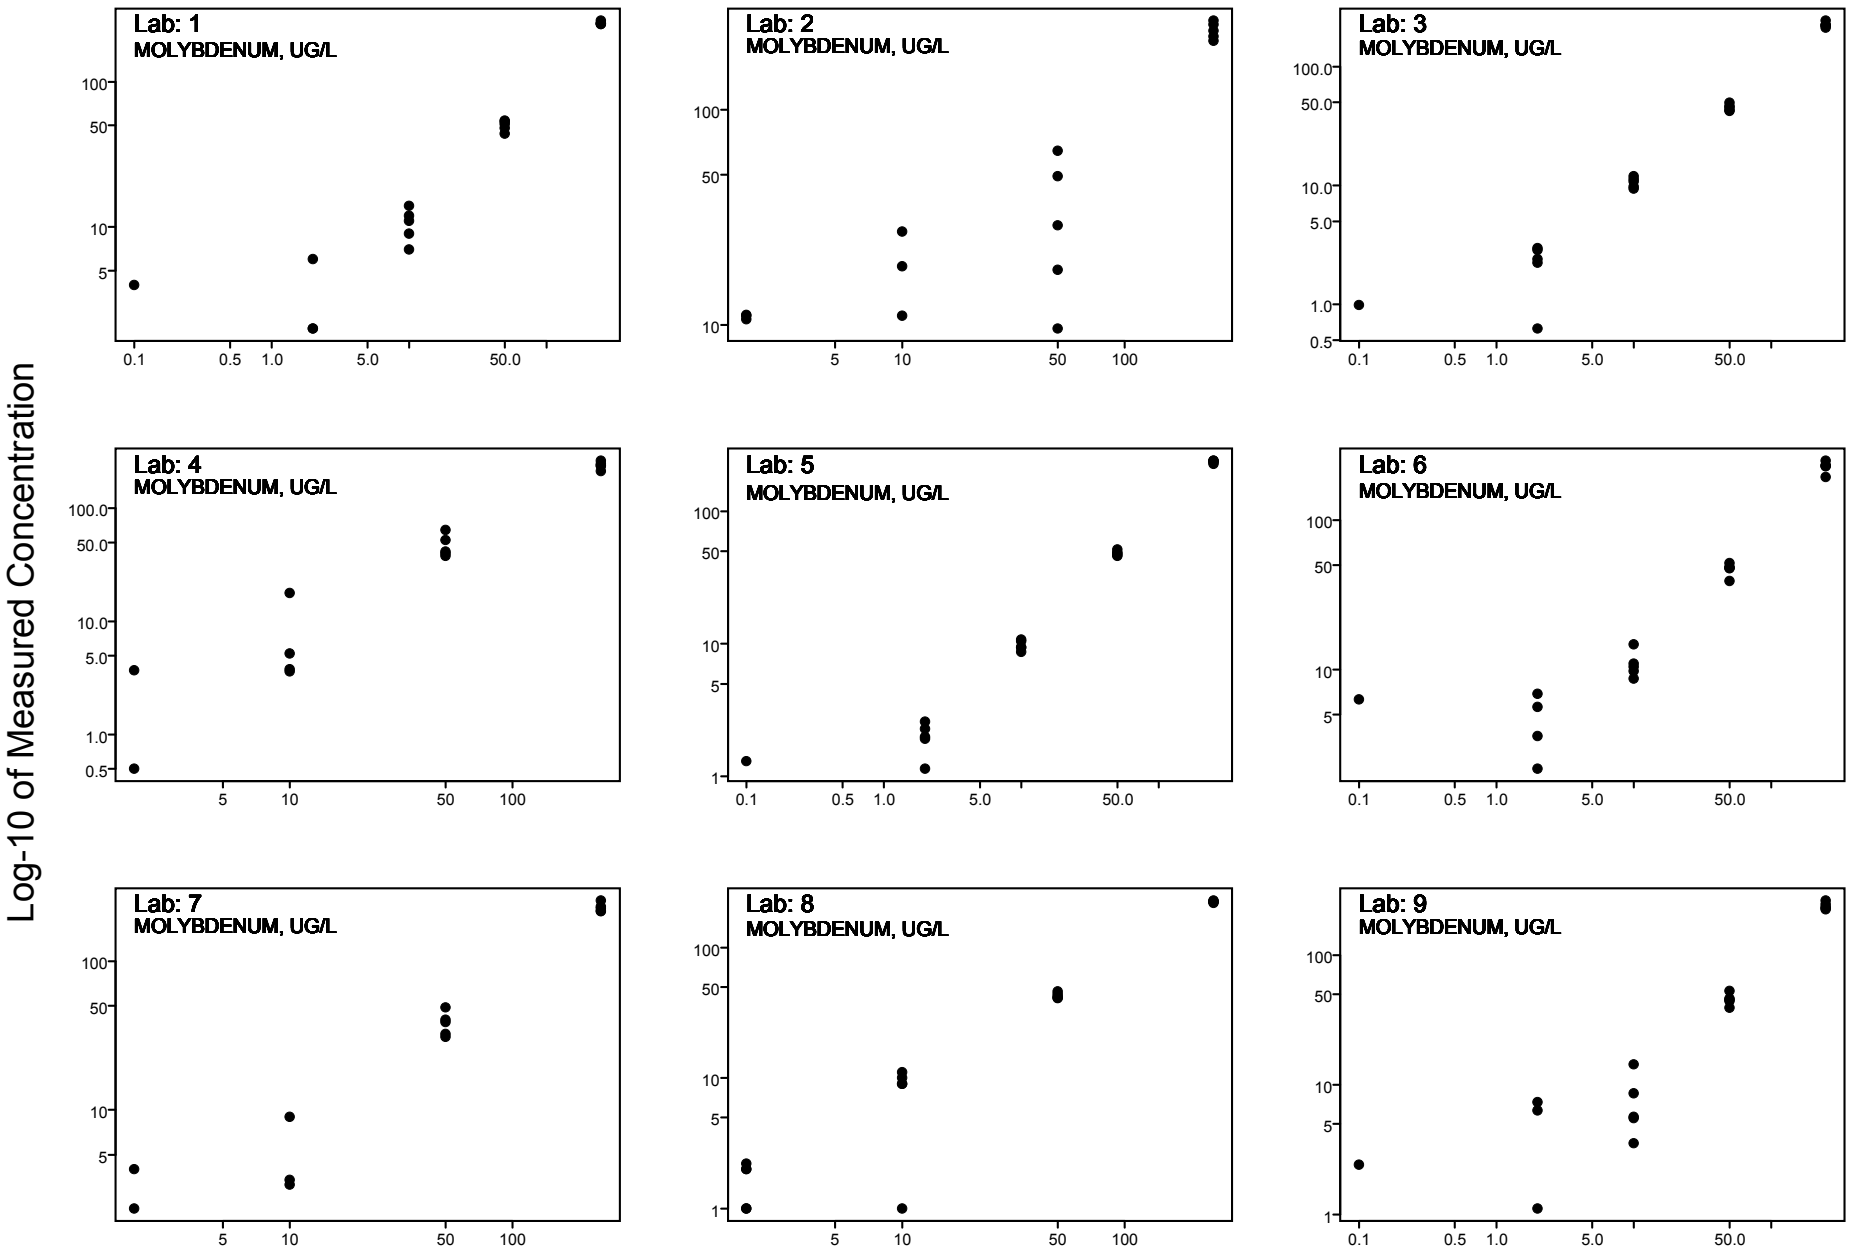

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

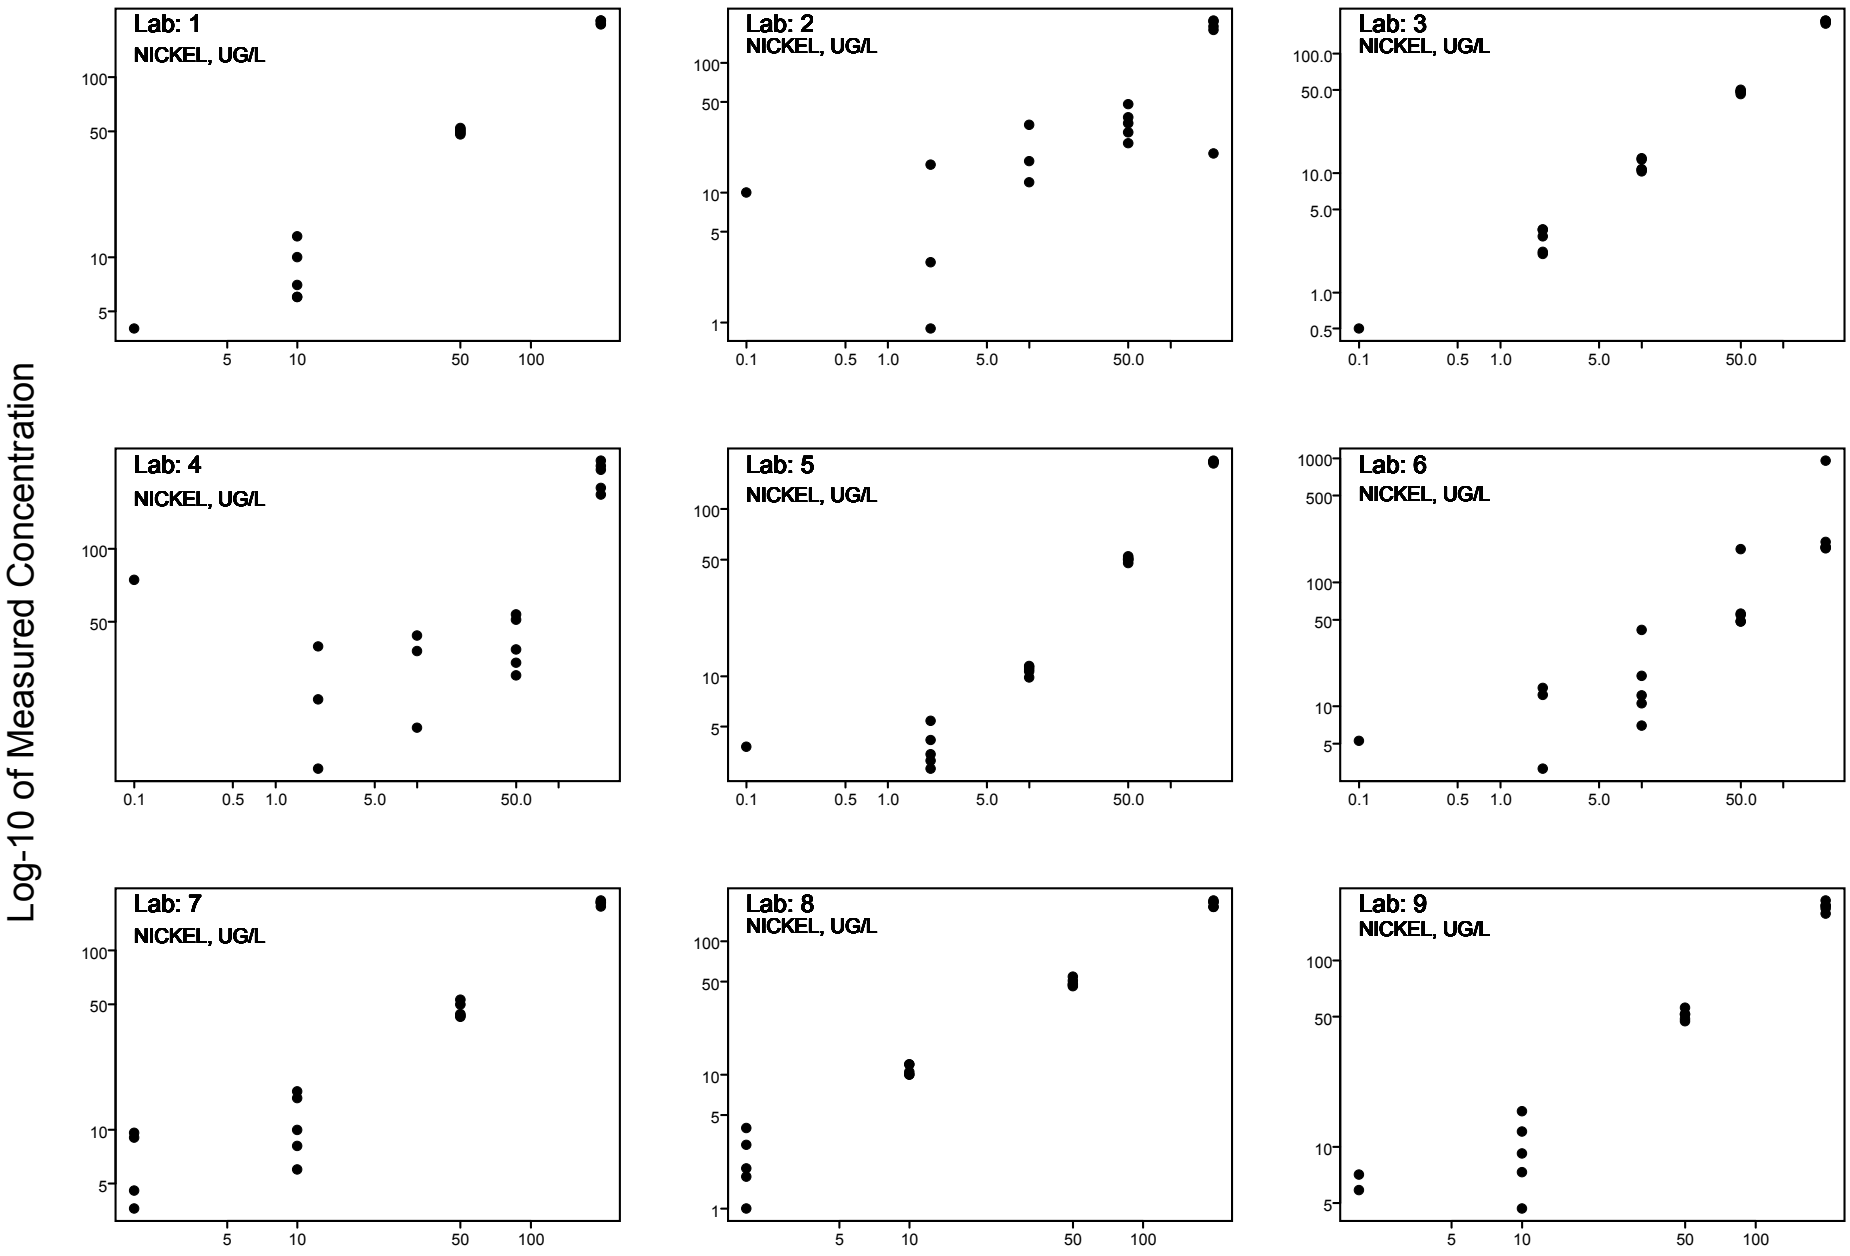

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

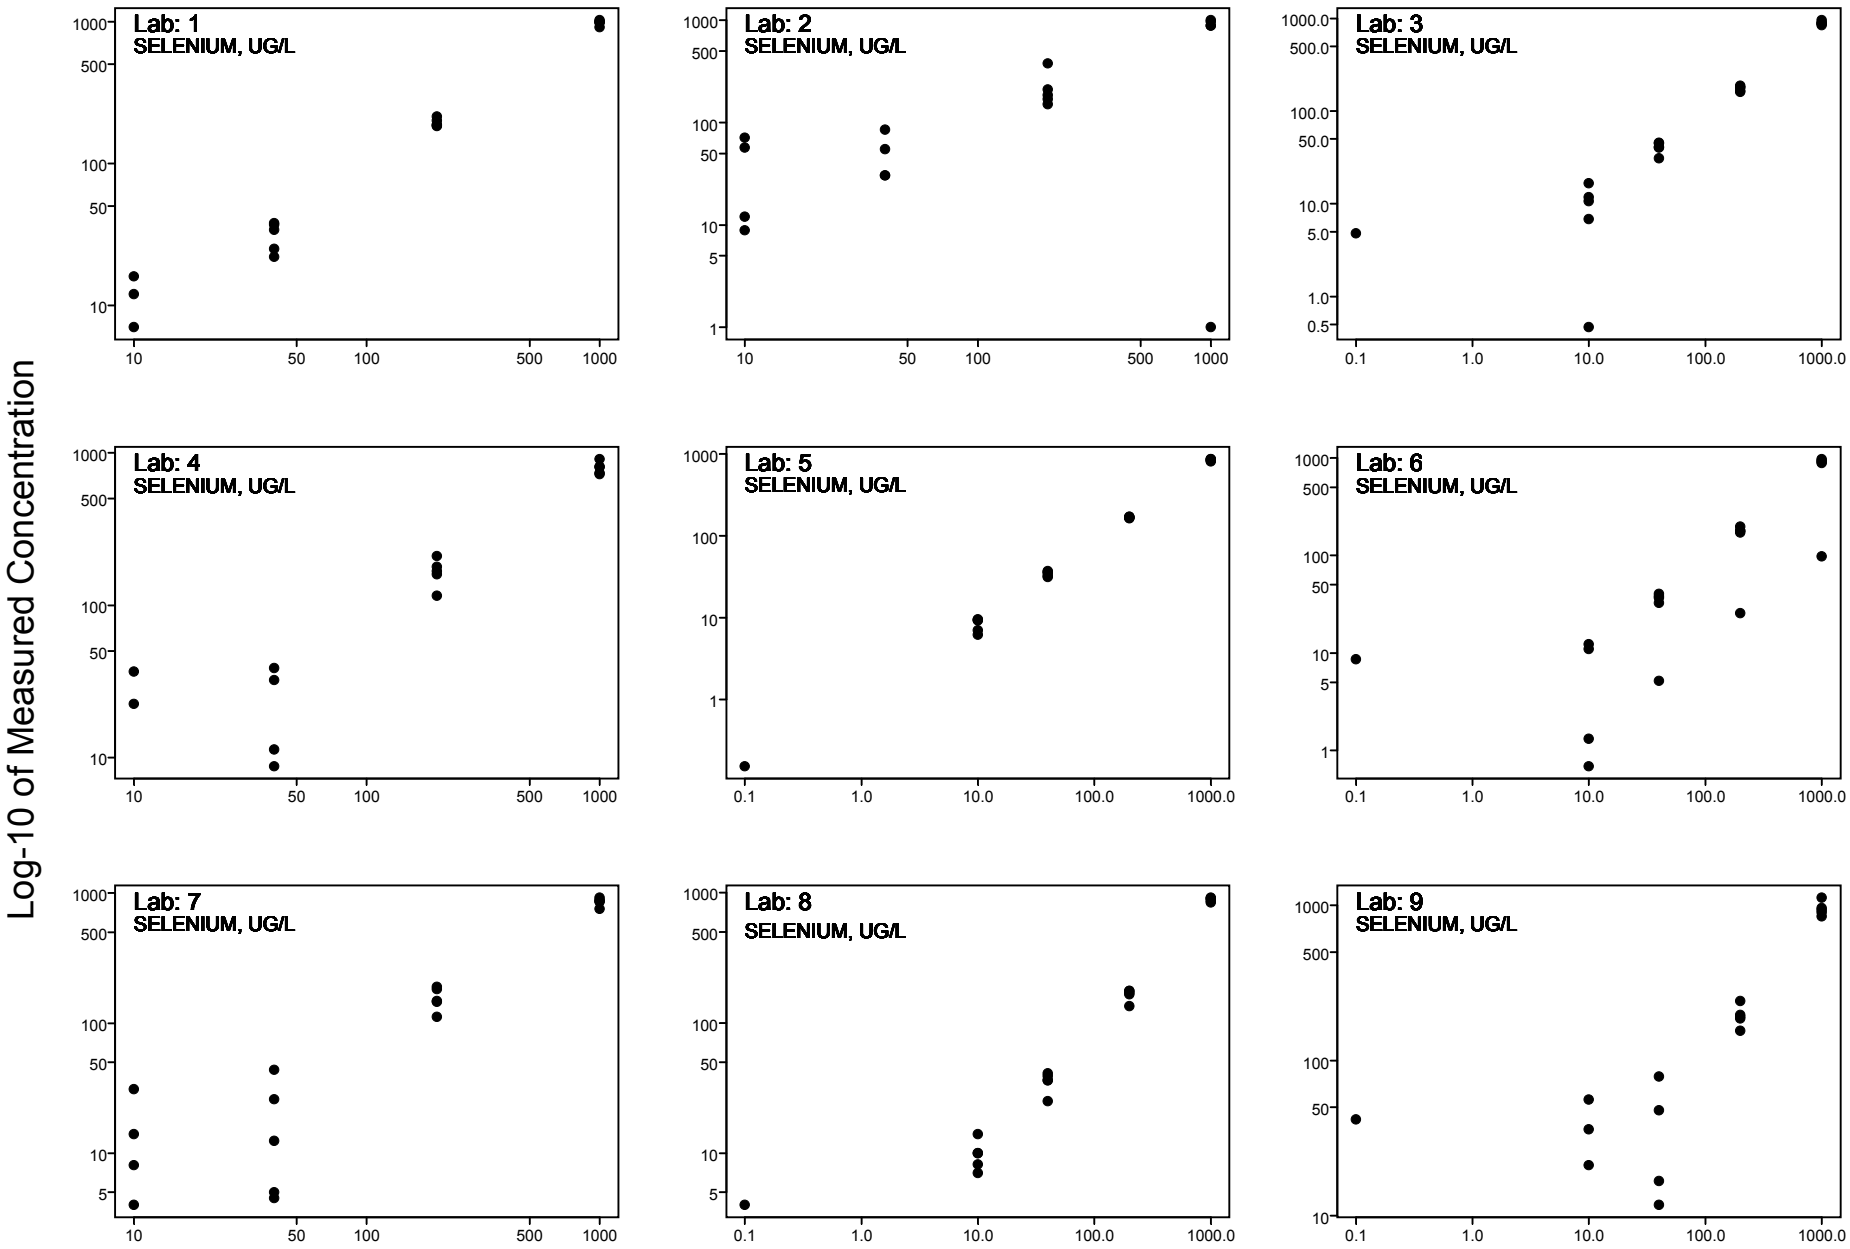

Measurement Results vs Spike Concentrations (Log-10 Scale)

(Matrix A, Method EPA 200.7 ICP/AES)

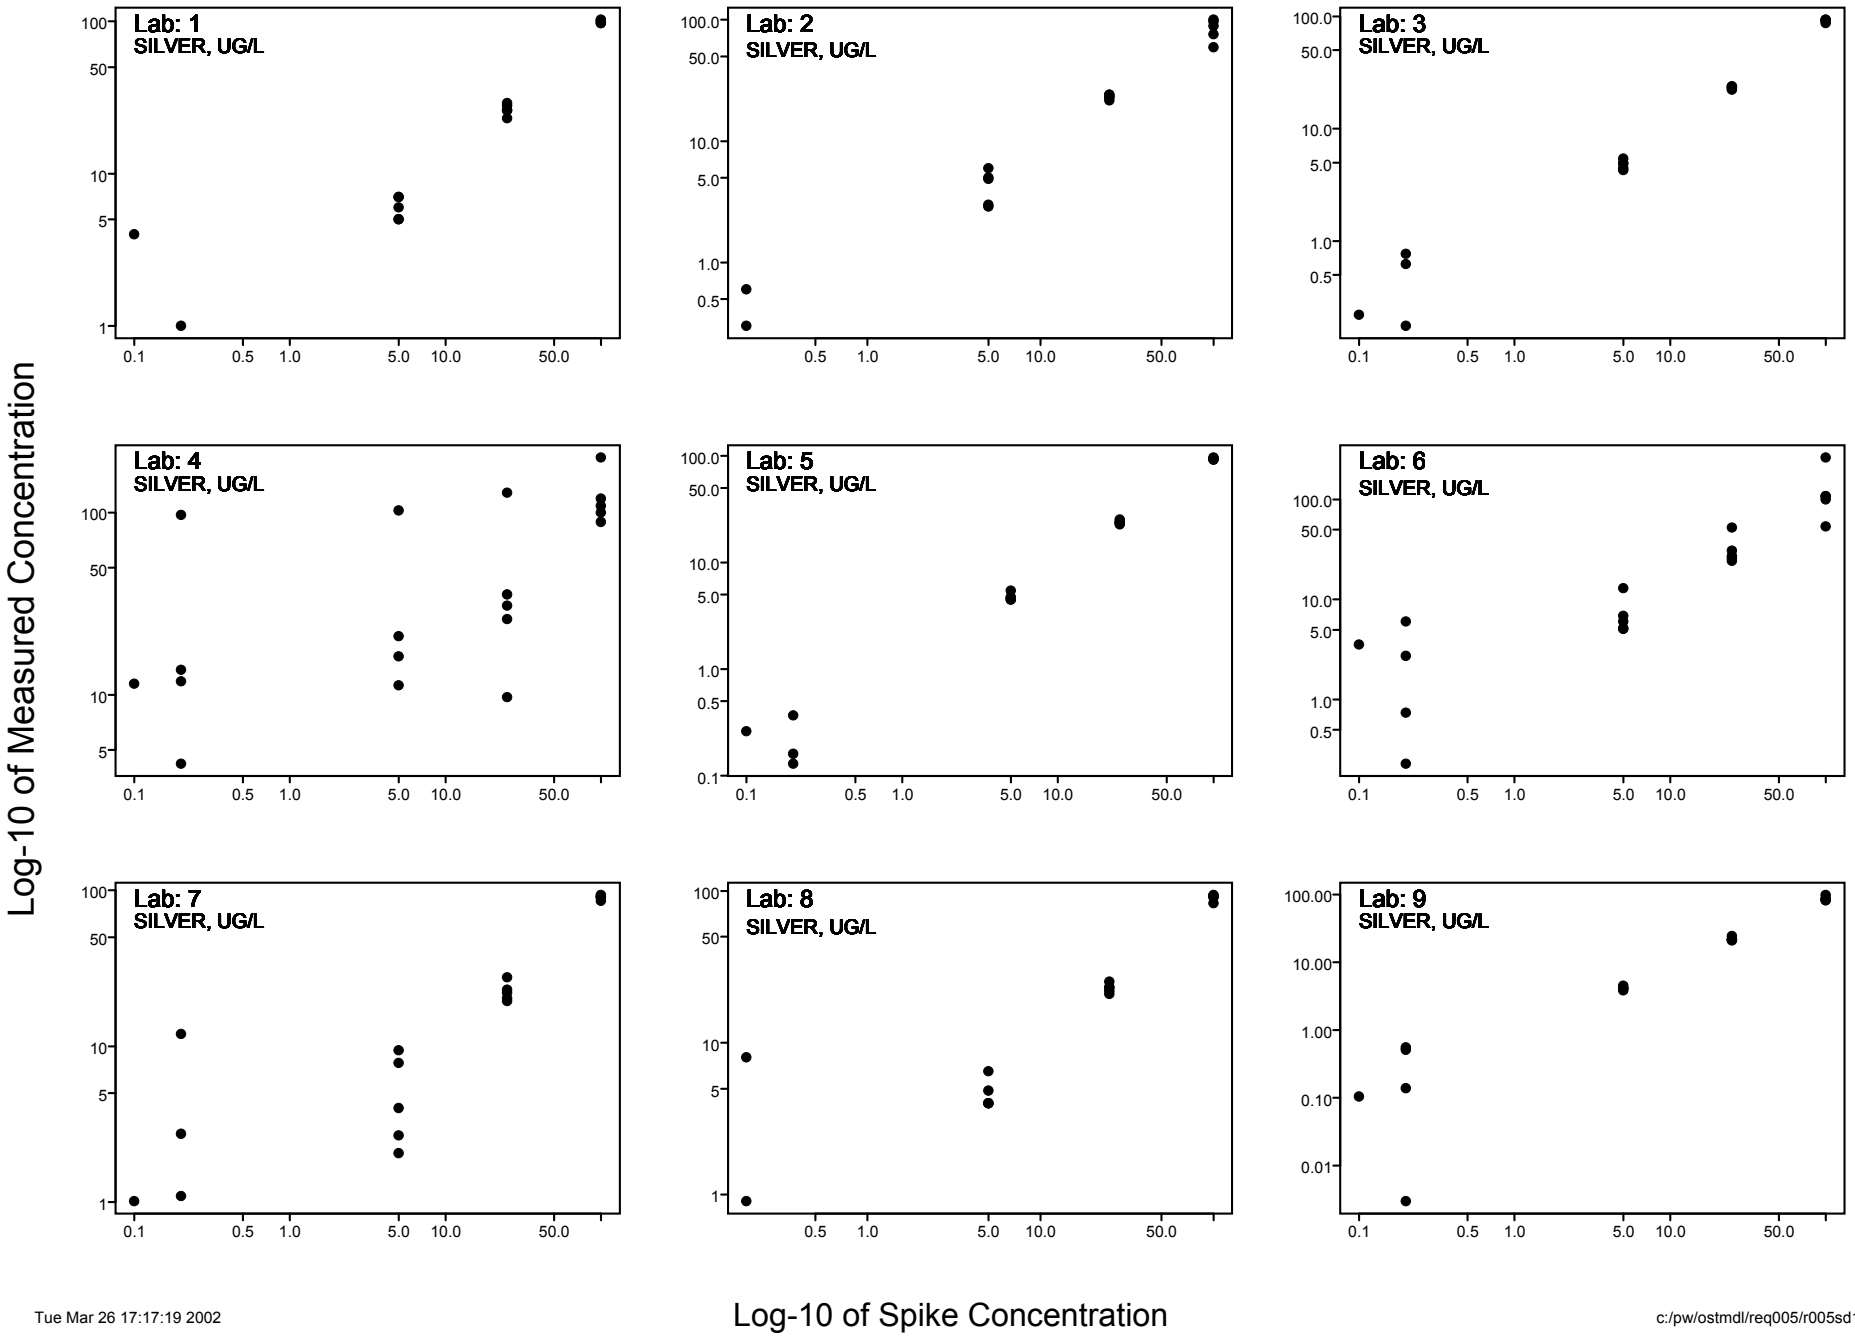

Measurement Results vs Spike Concentrations (Log-10 Scale)
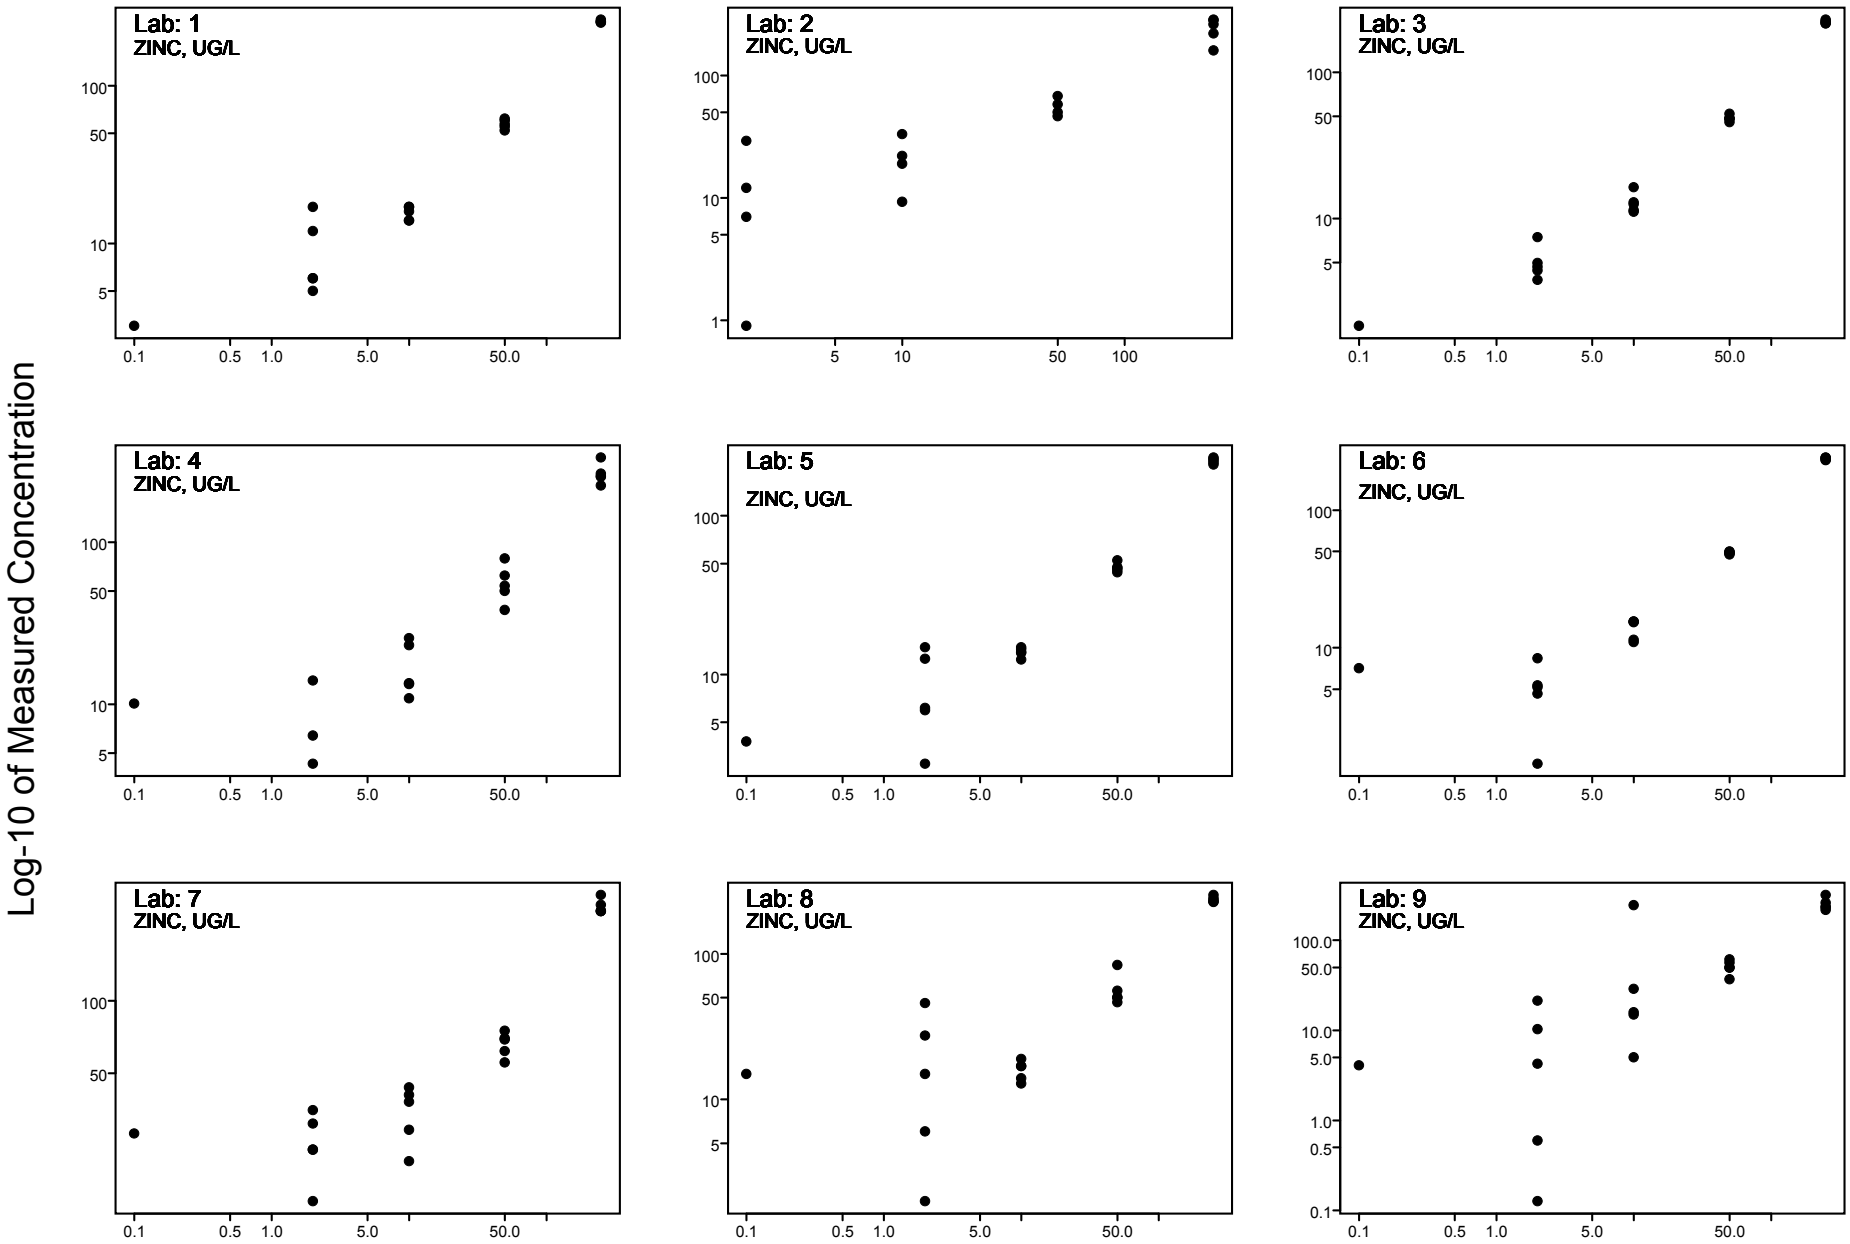
(Matrix A, Method EPA 200.7 ICP/AES)